


Sample Information

Order ID :GTA32412
 Name :N/A
 Sequence :LLGDFFRKSKEKIGKEFKRIVQRIKDFLRNLPRTES-NH2
 Lot. No :GTA32412-1030
 Pump A :0.1% Trifluoroacetic in 100% water
 Pump B :0.1% Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :SHIMADZU Inertsil ODS-SP(4.6*250mm*5um)
 Dissolution method :100% H2O
 Inj. Volume : 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	2
30.00	Pumps	B.Conc	65
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	2
50.00	Controller	Stop	

Chromatogram

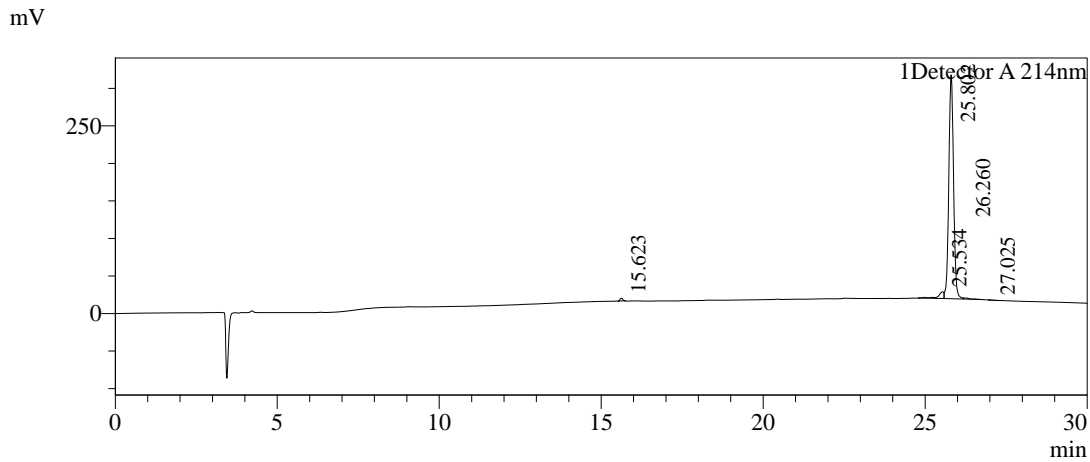

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	15.623	20469	3564	0.640
2	25.534	109960	8818	3.439
3	25.802	3042300	298187	95.159
4	26.260	19965	1478	0.624
5	27.025	4377	274	0.137
Total		3197071	312320	100.000