

CERTIFICATE OF ANALYSIS

Product Name	BMP-2 mimicking oligo peptide, Cat.#: 319721 (TFA removed)
Lot No.	P260724-CL1373116
Sequence	SSVPT-NH2 (Acetate salt)
Dissolution condition	100%H2O
Modification	Acetate salt
Molecular Weight (MW)	488.40
Storage	-20°C

Test Items	Specifications	Results
MW by MS	488.54	Conforms
Purity by HPLC	>95%	95.69%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Peptide content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	20mg	5mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Aug/12/2026


Quality Assurance Department



Sample Information

Order ID : N/A
 Name : BMP-2 mimicking oligo peptide, Cat.#: 319721 (TFA removed)
 Sequence : SSVPT-NH2 (Acetate salt)
 Lot. No : P260724-CL1373116
 Pump A : 0.1%TFA in 100%water
 Pump B : 0.1%TFA in 100%acetonitrile
 Total Flow : 1ml/min
 Wavelength : 220nm
 Analytical column type : 250*4.6mm,Boston Green ODS-AQ
 Dissolution method : 100%H2O

Chromatogram

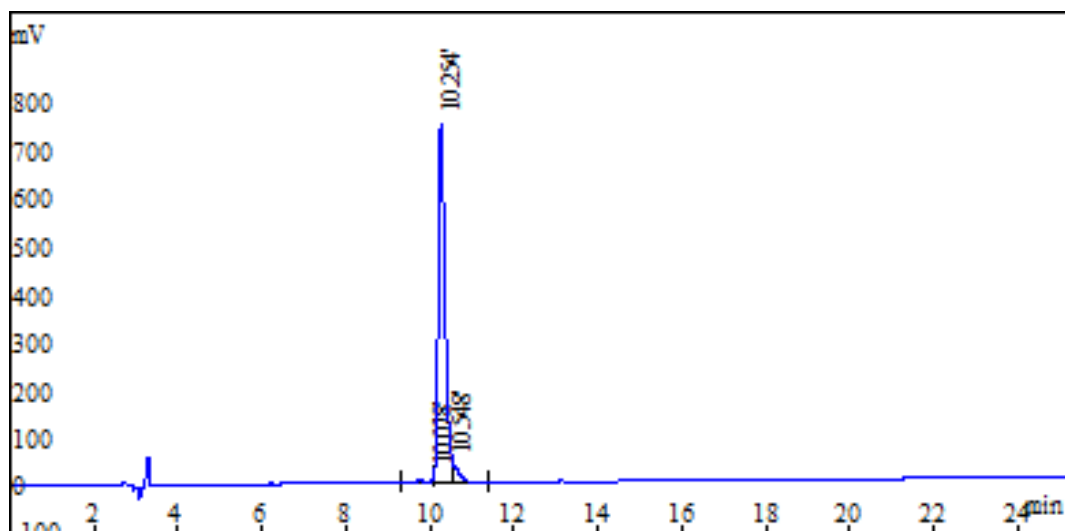


Peak Table

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.078	35664	9195	0.445
2	10.254	7669210	746757	95.69
3	10.548	309719	31753	3.864
Total	-	8014593	787705	100

MS Spectrum

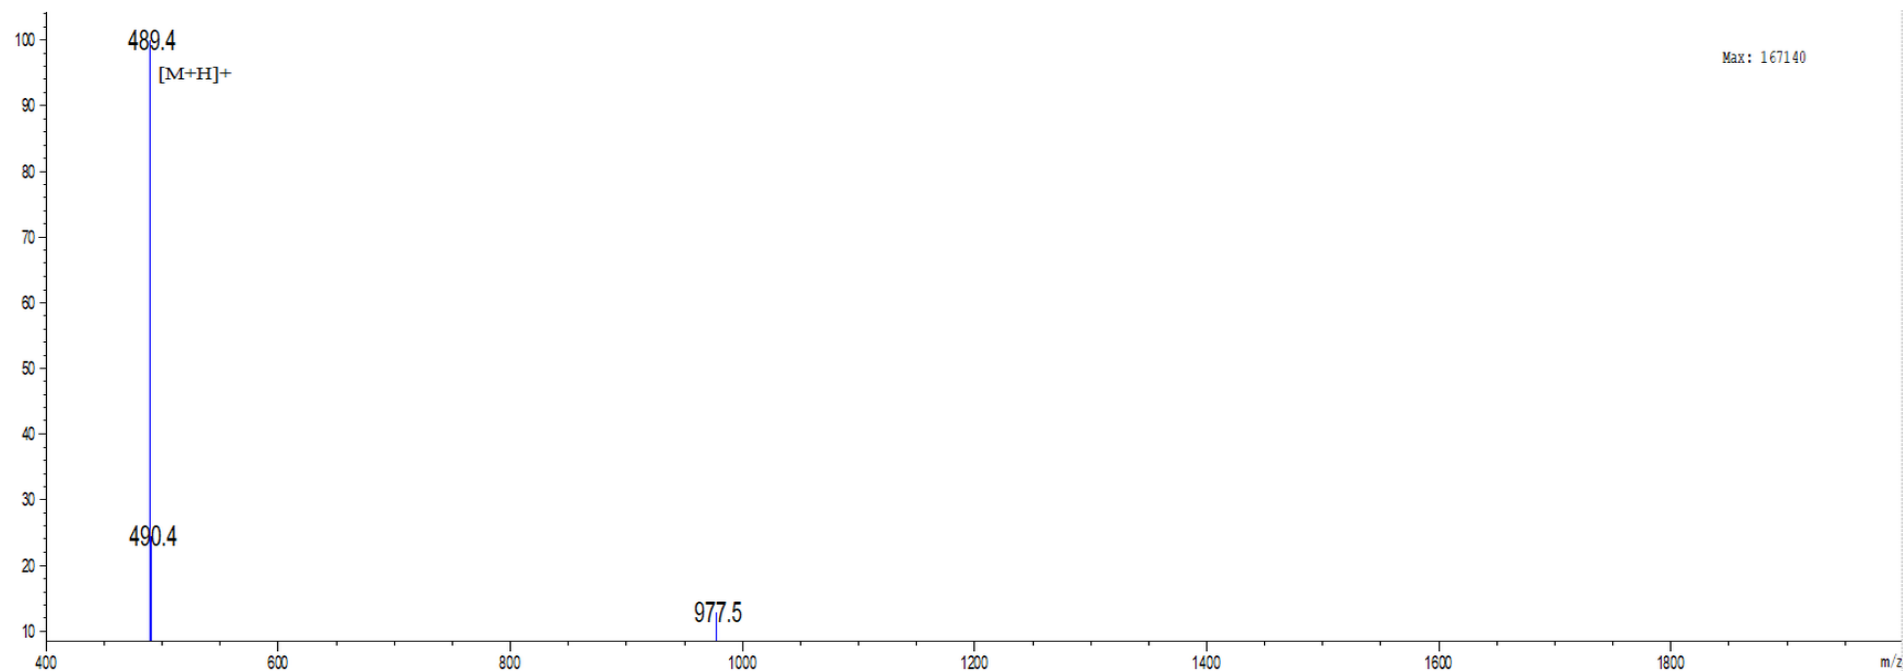

Sample Information

Date Acquired	: 2026/08/05	Interface	: ESI	Prerod Bias	: +4.5kv
Block Temp	: 200°C	Nebulizing Gas Flow	: 1.5L/min	Detector	: 1.5kv
Injection Volume	: 1ul	CDL Temp	: 250°C	T.Flow	: 0.2ml/min
		CDL Volt	: -20.0v	B.conc	: 50%H2O/50%ACN
Order ID	: N/A				
Name	: BMP-2 mimicking oligo peptide, Cat.#: 319721 (TFA removed)				
Sequence	: SSVPT-NH2 (Acetate salt)				
Lot.No	: P260724-CL1373116				
Theoretical	: 488.54				
Observed	: 488.40				