

## CERTIFICATE OF ANALYSIS

Product Name	BRP/BRINP2-related peptide, Cat.#: 319763 (TFA removed)
Lot No.	MTFA33535-251103
Sequence	THRILRRLFNLC-NH2 (Acetate Salt)
Dissolution condition	100%H2O
Modification	acetate salt
Molecular Weight (MW)	1540.87
Storage	-20°C

Test Items	Specifications	Results
MW by MS	1540.95	Conforms
Purity by HPLC	>95%	97.116%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	100 mg	5.0mg*20

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Nov/07/2025

Quality Assurance Department




### Sample Information

Order ID	:MTFA33535		
Name	:BRP/BRINP2-related peptide		
Sequence	:THRILRRLFNLC-NH2 (Acetate Salt)		
Lot. No	:MTFA33535-251103		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 µm)		
Dissolution method	:100%H2O		
Inj. Volume	: 25ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	20
30.00	Pumps	B.Conc	50
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	20
50.00	Controller	Stop	

### Chromatogram

mV

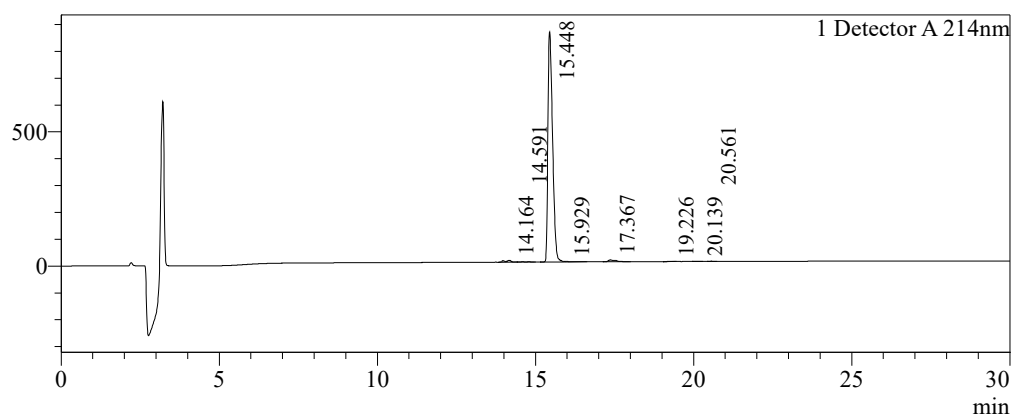


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	14.164	89969	6870	0.995
2	14.591	15407	1102	0.170
3	15.448	8783895	856883	97.116
4	15.929	31534	1810	0.349
5	17.367	112876	6886	1.248
6	19.226	2208	241	0.024
7	20.139	1918	214	0.021
8	20.561	6959	925	0.077
Total		9044767	874933	100.000

# MS Spectrum

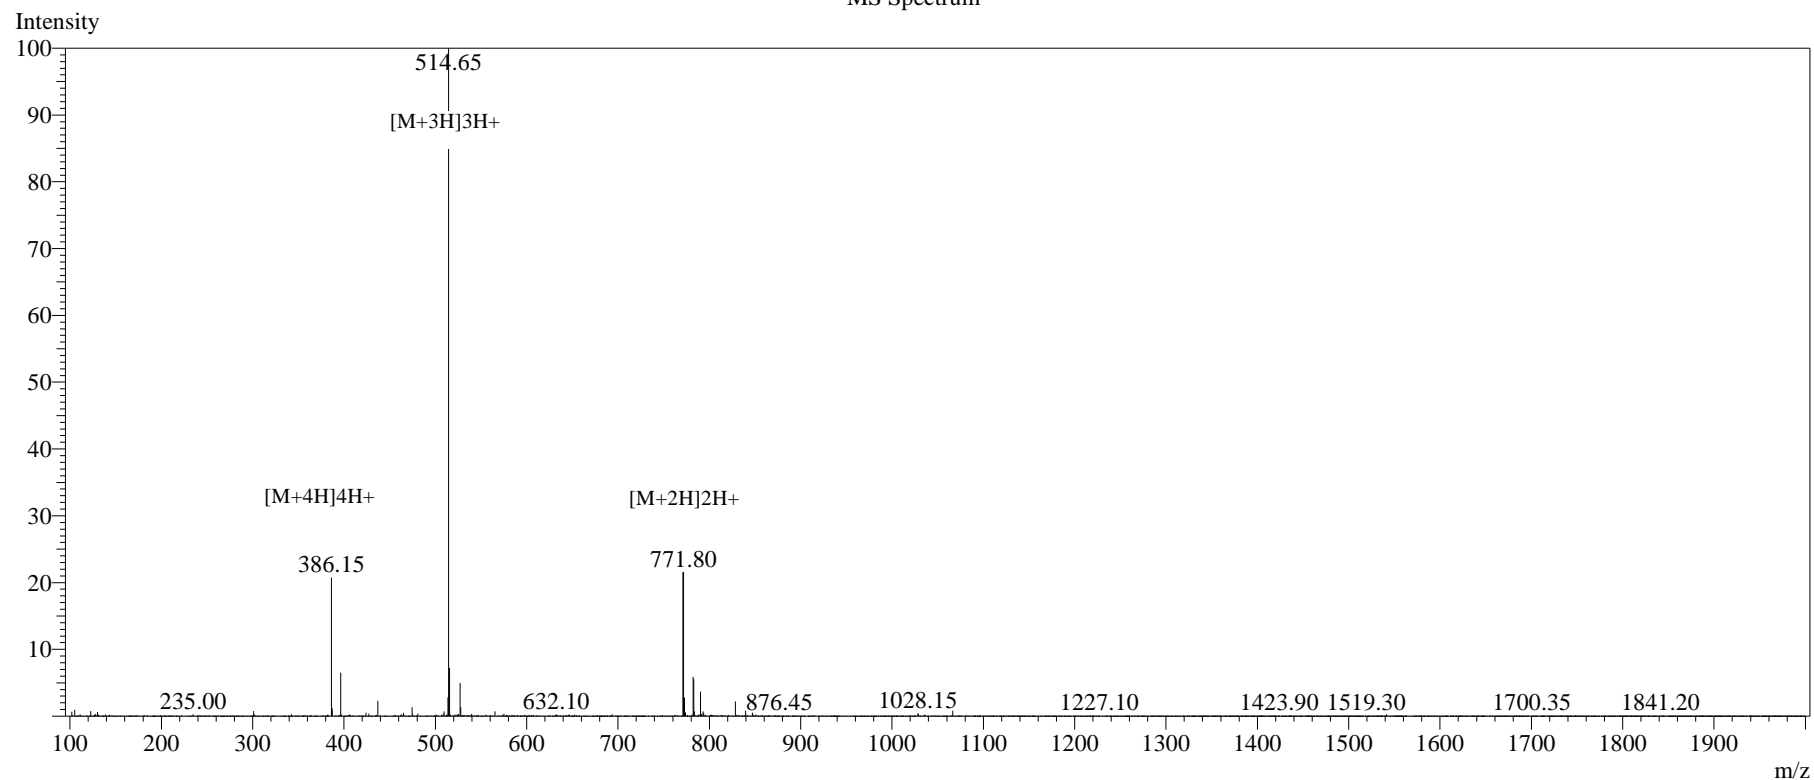

## Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/11/03 16:17:35	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% ME OH
Order ID	:MTFA33535				
Name	:BRP/BRINP2-related peptide				
Sequence	:THRILRRLFNLC-NH <sub>2</sub> (Acetate Salt)				
Lot.No	:MTFA33535-251103				
Theoretical	:1540.87				
Observed	:1540.95				