

CERTIFICATE OF ANALYSIS

Product Name	DALDA peptide, Cat.#: 319553
Lot No.	MTFA31964-1016
Sequence	YrFK
Dissolution condition	100%H2O
Length	4AA
Modification	r=D-Arg
Molecular Weight (MW)	612.72
Storage	-20°C

Test Items	Specifications	Results
MW by MS	612.70	Conforms
Purity by HPLC	>95%	99.770%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	20mg	5.0mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Oct/28/2024




Sample Information

Order ID :MTFA31964
 Name :DALDA peptide
 Sequence :YrFK
 Lot. No :MTFA31964-1016
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Kromasil 100-5-C18 (4.6*250mm*5 µm)
 Dissolution method :100%H2O
 Inj. Volume : 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	0.1
30.00	Pumps	B.Conc	30
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	0.1
50.00	Controller	Stop	

Chromatogram

mV

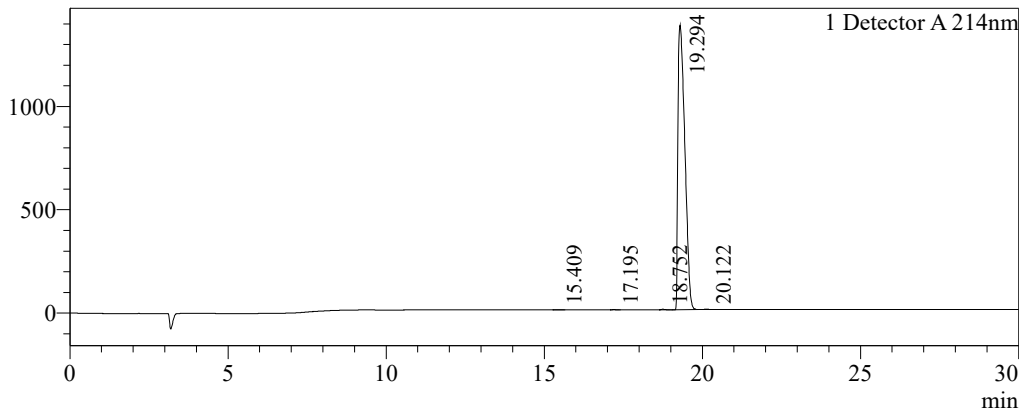


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	15.409	4450	474	0.021
2	17.195	9857	1460	0.047
3	18.752	18085	2610	0.086
4	19.294	21002534	1376345	99.770
5	20.122	16062	2132	0.076
Total		21050987	1383021	100.000

MS Spectrum

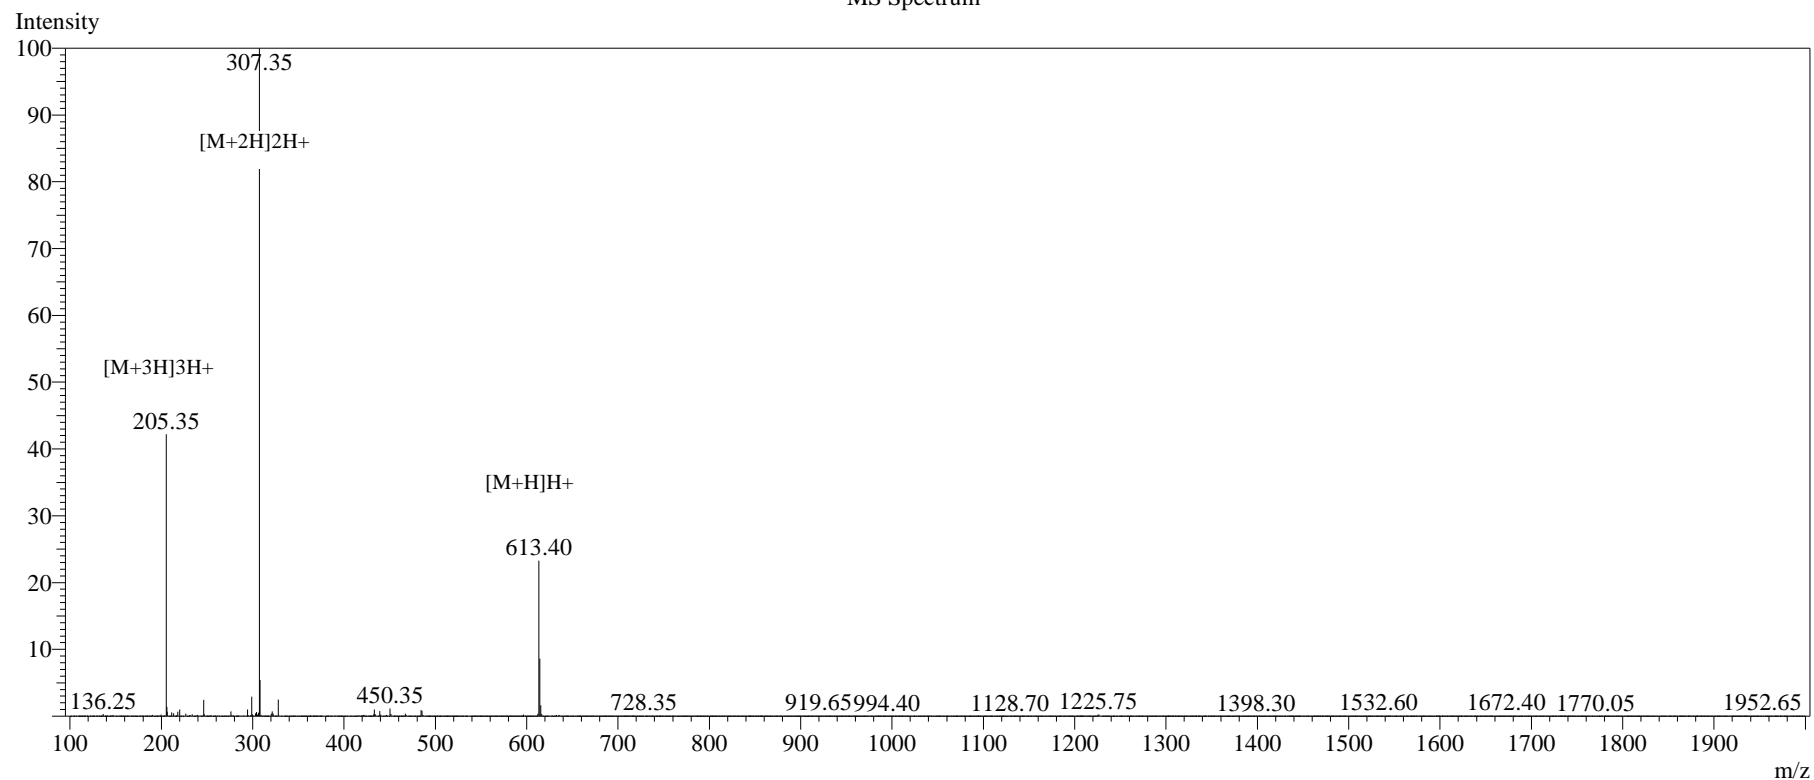

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/10/25 11:41:34	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% MEOH

Order ID	:MTFA31964
Name	:DALDA peptide
Sequence	:YrFK
Lot.No	:MTFA31964-1016
Theoretical	:612.72
Observed	:612.70