
CERTIFICATE OF ANALYSIS

Product Name	DrkBiT, Cat.#: 319394 (TFA removed)
Lot No.	MTFB21199-261008
Sequence	VSGWALFKKIS (Acetate Salt)
Dissolution condition	100%H ₂ O
Modification	Acetate salt
Molecular Weight (MW)	1235.48
Storage	-20°C

Test Items	Specifications	Results
MW by MS	1235.25	Conforms
Purity by HPLC	>95%	98.444%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Peptide content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	150.0mg	5.0mg*30

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Oct/22/2026


Quality Assurance Department



Sample Information

Order ID	:MTFB21199		
Name	:DrkBiT, Cat.#: 319394 (TFA removed)		
Sequence	:VSGWALFKKIS (Acetate Salt)		
Lot. No	:MTFB21199-261008		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 µm)		
Dissolution method	:100%H2O		
Inj. Volume	: 10ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	15
30.00	Pumps	B.Conc	45
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	15
50.00	Controller	Stop	

Chromatogram

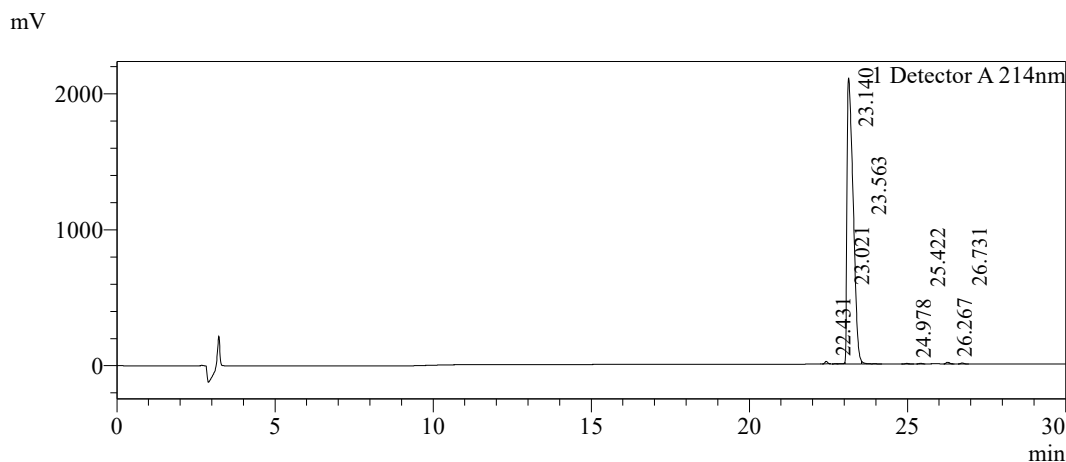


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	22.431	108118	17724	0.374
2	23.021	51053	6810	0.177
3	23.140	28453472	2100121	98.444
4	23.563	100735	18386	0.349
5	24.978	23453	3608	0.081
6	25.422	28001	3776	0.097
7	26.267	90014	12049	0.311
8	26.731	48270	6976	0.167
Total		28903115	2169450	100.000

MS Spectrum

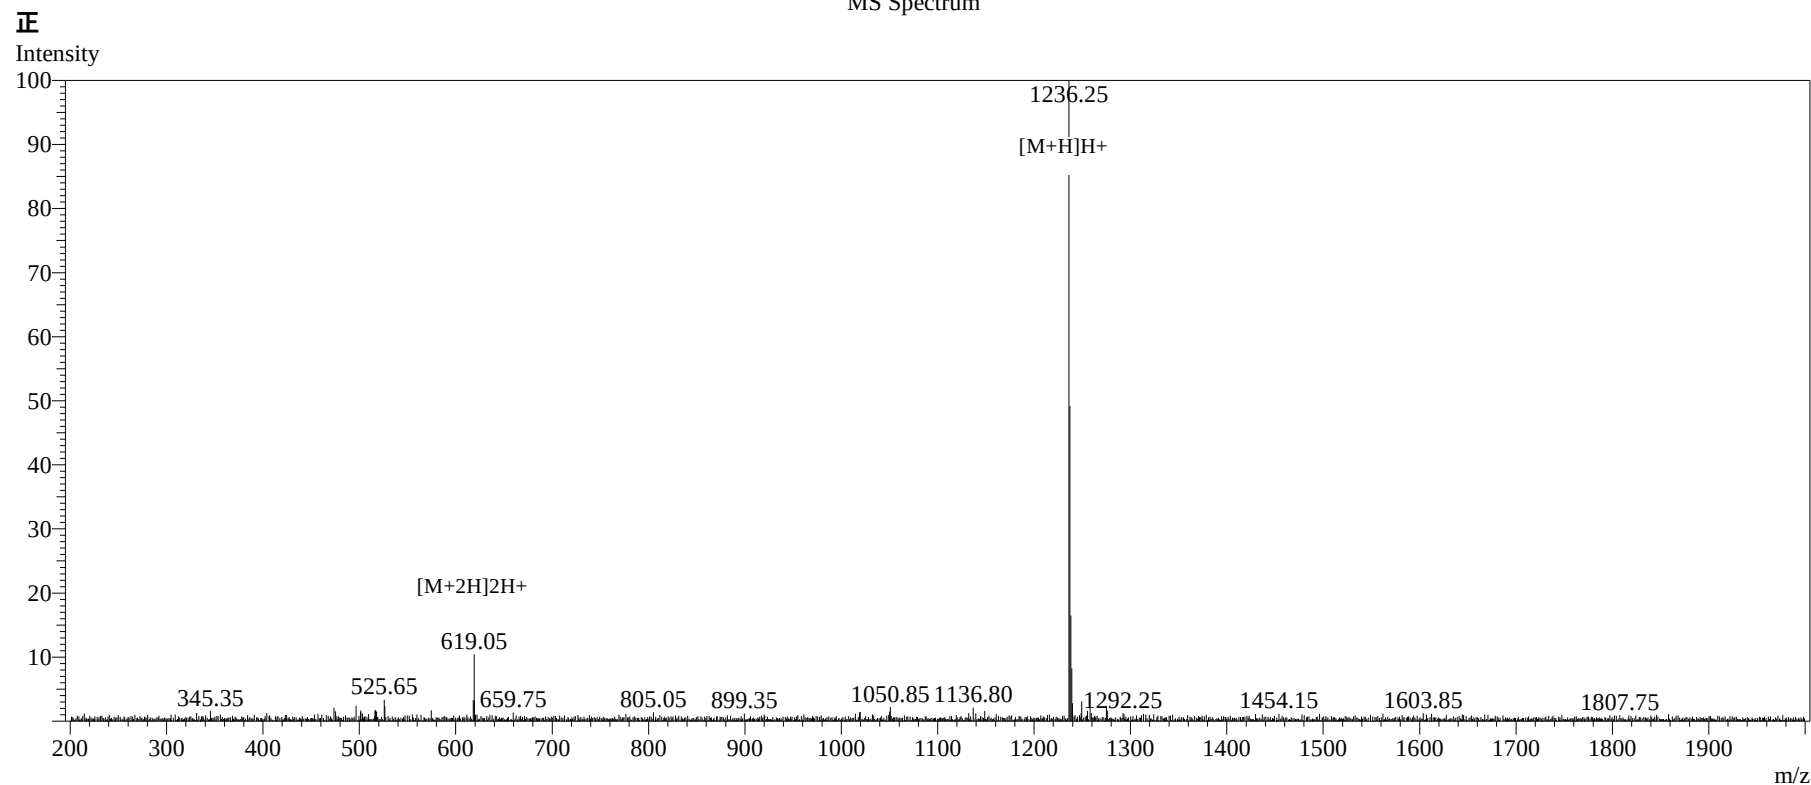

Sample Information

Dissolution method	:15%ACN+85%H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2026/10/21 13:37:30	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H ₂ O/50%MEOH

Order ID	:MTFB21199
Name	:DrkBiT, Cat.#: 319394 (TFA removed)
Sequence	:VSGWALFKKIS (Acetate Salt)
Lot.No	:MTFB21199-261008
Theoretical	:1235.48
Observed	:1235.25