

CERTIFICATE OF ANALYSIS

Product Name Pigment-dispersing factor, Drm-PDH peptide, Cat.#: 315085

Lot No. MTFA32136-1125

Sequence NSELINSLLSLPKNMNDA-NH2

Dissolution condition 100%H2O

Length 18AA

Modification N/A

Molecular Weight (MW) 1972.20

Storage -20°C

Test Items	Specifications	Results
MW by MS	1972.50	Conforms
Purity by HPLC	>95%	98.819%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	10mg	5.0mg*2

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:

Dec/09/2024



Sample Information

Order ID :MTFA32136 Name :Drm-PDH

Sequence :NSELINSLLSLPKNMNDA-NH2

Lot. No :MTFA32136-1125

Pump A :0.1%Trifluoroacetic in 100% water Pump B :0.1%Trifluoroacetic in 100% acetonitrile

Total Flow :1ml/min Wavelength :214nm


Analytial column type :Kromasil 100-5-C18 (4.6*250mm*5 μm)

Dissolution method :100%H2O

Inj. Volume : 25ul Time Module Action Value 0.01 **Pumps** B.Conc 25 55 30.00 Pumps B.Conc 33.00 Pumps B.Conc 100 38.00 B.Conc 100 Pumps 25 40.00 Pumps B.Conc 50.00 Controller Stop

Chromatogram

mV

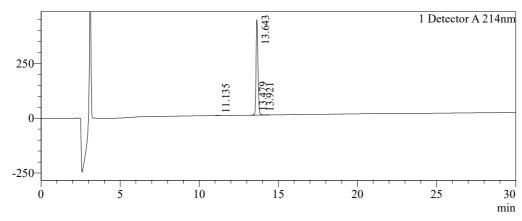

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%		
1	11.135	3841	452	0.105		
2	13.479	16031	3530	0.440		
3	13.643	3602368	433410	98.819		
4	13.921	23191	2535	0.636		
Total		3645431	439928	100.000		




:+4.5kv :-0.2kv

:0.2ml/min

:50%H2O/50%MEOH

MS Spectrum

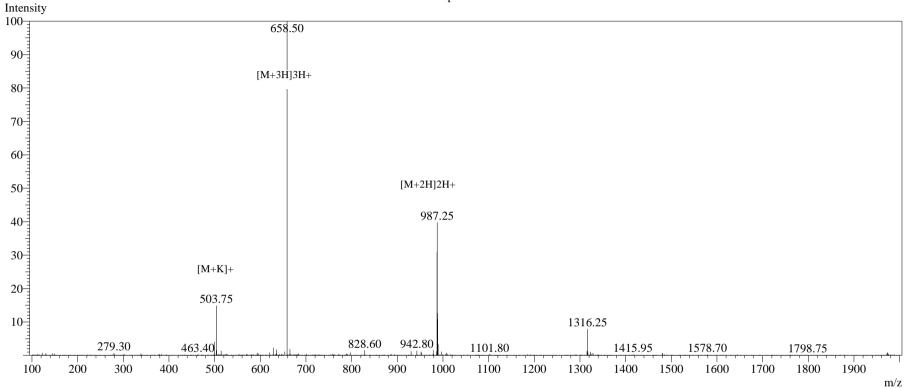

Sample Information

Dissolution method	:15%ACN+85%H2O	Interface	:ESI :1.50L/min	Prerod Bias Detector
Date Acquired	:2024/12/06 13:16:05	Nebulizing Gas Flow	:1.30L/IIIII	
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow
Block Temp	:200	CDL Volt	:0v	B.conc

Order ID :MTFA32136 :Drm-PDH Name

Sequence Lot.No :NSELINSLLSLPKNMNDA-NH2

:MTFA32136-1125 :1972.20 :1972.50

Theoretical Observed