

**CERTIFICATE OF ANALYSIS**

<b>Product Name</b>	Eumenitin peptide, Cat.# 310731
<b>Lot No.</b>	GTA34558-2-0920
<b>Sequence</b>	LNLKGIFKKVASLLT
<b>Dissolution condition</b>	100%H2O
<b>Length</b>	15AA
<b>Modification</b>	N/A
<b>Molecular Weight (MW)</b>	1645.03
<b>Storage</b>	-20°C

<b>Test Items</b>	<b>Specifications</b>	<b>Results</b>
<b>MW by MS</b>	1645.20	Conforms
<b>Purity by HPLC</b>	>95%	96.851%
<b>Peptide Content</b>	N/A	N/A
<b>Moisture content</b>	N/A	N/A
<b>Acetic acid content</b>	N/A	N/A
<b>Appearance</b>	White to off-white lyophilized powder	Conforms
<b>Quantity</b>	10mg	5.0mg*2

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Sep/28/2022




### Sample Information

Order ID :GTA34558-2  
 Name :Eumenitin peptide  
 Sequence :LNLKGIFKKVASLLT  
 Lot. No :GTA34558-2-0920  
 Pump A :0.1% Trifluoroacetic in 100% water  
 Pump B :0.1% Trifluoroacetic in 100% acetonitrile  
 Total Flow :1ml/min  
 Wavelength :214nm  
 Analytical column type :YMC-Triart C18(4.6\*250mm\*5um)  
 Dissolution method :100% H2O  
 Inj. Volume : 40ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	30
30.00	Pumps	B.Conc	60
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	30
50.00	Controller	Stop	

### Chromatogram

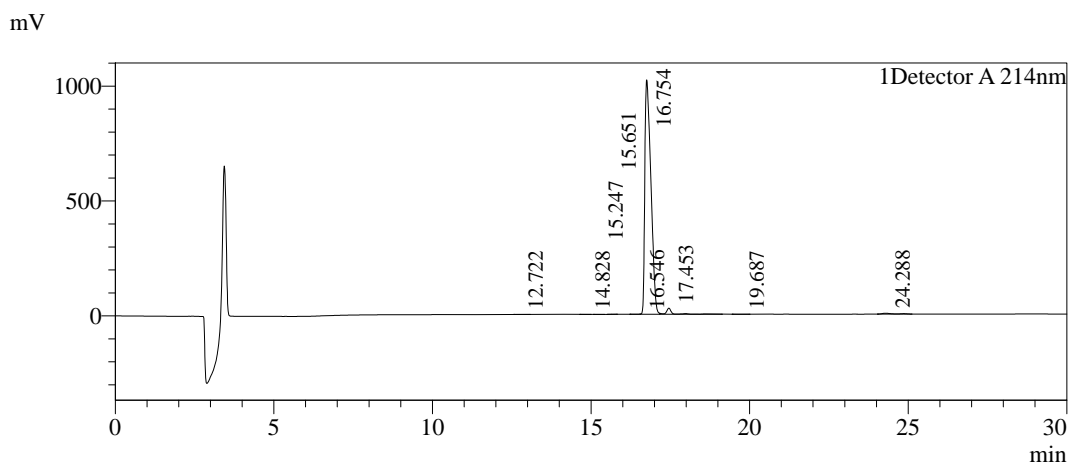


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	12.722	4384	396	0.031
2	14.828	4240	538	0.030
3	15.247	3663	514	0.026
4	15.651	5576	660	0.040
5	16.546	4681	578	0.033
6	16.754	13629762	1020046	96.851
7	17.453	322984	26372	2.295
8	19.687	4100	280	0.029
9	24.288	93478	3780	0.664
Total		14072868	1053164	100.000

## MS Spectrum

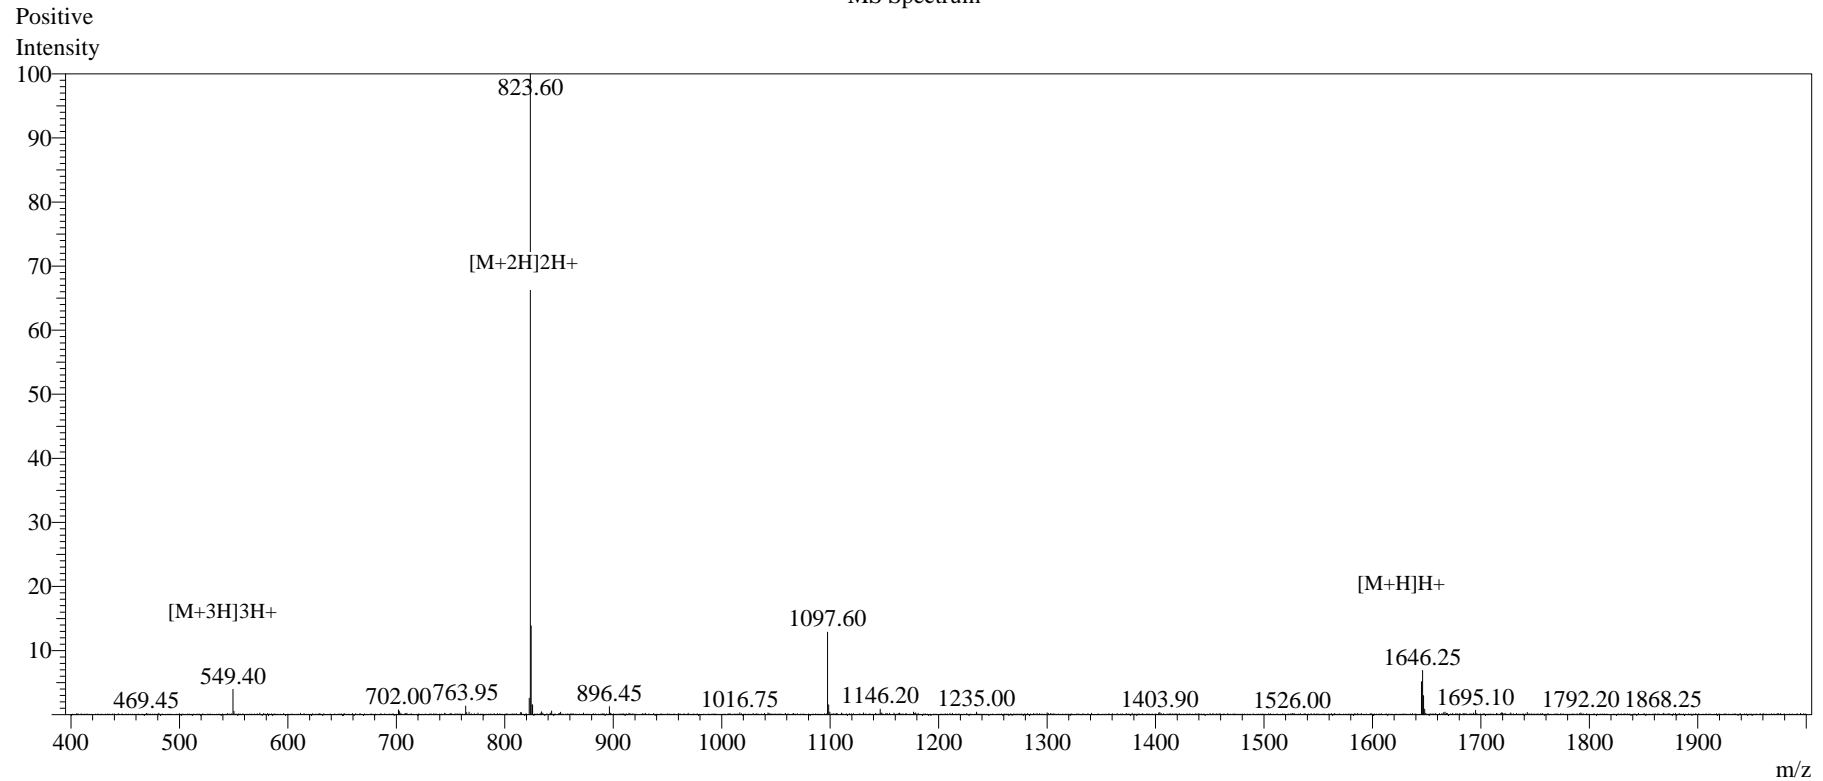

## Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2022/09/28 14:24:42	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% MEOH

Order ID	:GTA34558-2
Name	:Eumenitin peptide
Sequence	:LNLKGIFKKVASLLT
Lot.No	:GTA34558-2-0920
Theoretical	:1645.03
Observed	:1645.20