

## CERTIFICATE OF ANALYSIS

<b>Product Name</b>	GFOGER peptide, Cat.#: 319307
<b>Lot No.</b>	MTFA31689-0812
<b>Sequence</b>	GFOGER
<b>Dissolution condition</b>	100%H2O
<b>Length</b>	6AA
<b>Modification</b>	O=Hyp
<b>Molecular Weight (MW)</b>	677.71
<b>Storage</b>	-20°C

<b>Test Items</b>	<b>Specifications</b>	<b>Results</b>
<b>MW by MS</b>	677.70	Conforms
<b>Purity by HPLC</b>	>95%	95.809%
<b>Peptide content</b>	N/A	N/A
<b>Moisture content</b>	N/A	N/A
<b>Acetic acid content</b>	N/A	N/A
<b>Appearance</b>	White to off-white lyophilized powder	Conforms
<b>Quantity</b>	20mg	5.0mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Aug/27/2024




Sample Information

Order ID :MTFA31689  
 Name :GFOGER peptide  
 Sequence :GFOGER  
 Lot. No :MTFA31689-0812  
 Pump A :0.1%Trifluoroacetic in 100% water  
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile  
 Total Flow :1ml/min  
 Wavelength :214nm  
 Analytical column type :Kromasil 100-5-C18 (4.6\*250mm\*5 µm)  
 Dissolution method :100%H2O  
 Inj. Volume : 20ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	5
30.00	Pumps	B.Conc	35
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	5
50.00	Controller	Stop	

Chromatogram

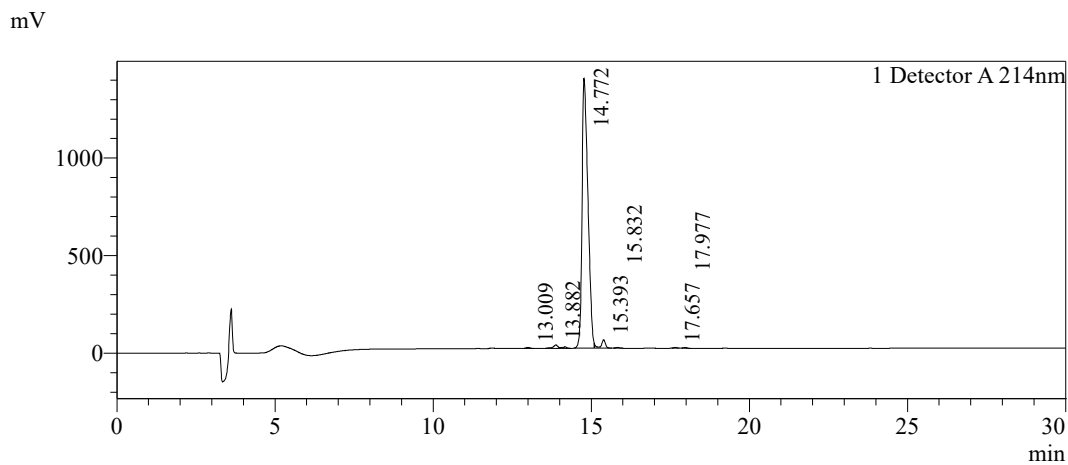


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	13.009	37045	4769	0.198
2	13.882	254551	17489	1.361
3	14.772	17920735	1382734	95.809
4	15.393	419340	43193	2.242
5	15.832	27848	4234	0.149
6	17.657	22521	3660	0.120
7	17.977	22636	3397	0.121
Total		18704675	1459476	100.000

### MS Spectrum

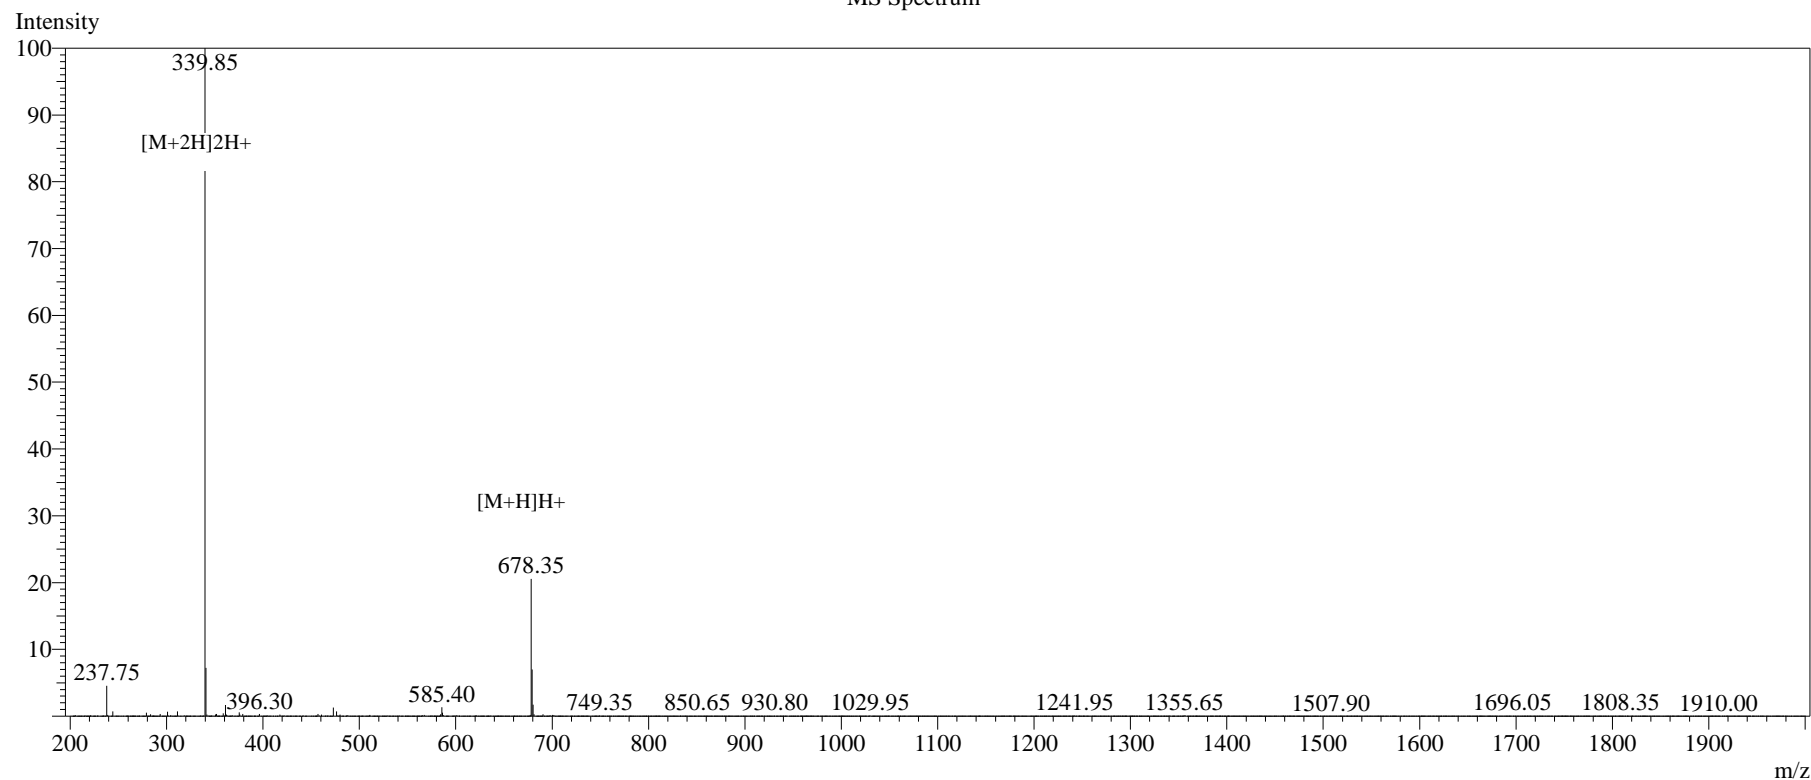

### Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/08/13 10:30:59	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% MEOH

Order ID	:MTFA31689
Name	:GFOGER peptide
Sequence	:GFOGER
Lot.No	:MTFA31689-0812
Theoretical	:677.71
Observed	:677.70