

---

**CERTIFICATE OF ANALYSIS**

<b>Product Name</b>	human Histatin 1 peptide, Cat.#: 301359
<b>Lot No.</b>	MTFB20521-01-260130
<b>Sequence</b>	DSHEKRHHGYRRKFHEKHHSHREFPFYGDYGSNYLYDN
<b>Dissolution condition</b>	100%H2O
<b>Modification</b>	N/A
<b>Molecular Weight (MW)</b>	4848.13
<b>Storage</b>	-20°C

---

<b>Test Items</b>	<b>Specifications</b>	<b>Results</b>
<b>MW by MS</b>	4848.90	Conforms
<b>Purity by HPLC</b>	>95%	96.993%
<b>Endotoxin Content</b>	N/A	N/A
<b>TFA solubility</b>	N/A	N/A
<b>Moisture content</b>	N/A	N/A
<b>Acetic acid content</b>	N/A	N/A
<b>Appearance</b>	White to off-white lyophilized powder	Conforms
<b>Quantity</b>	10 mg	5.0mg*2

---

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Mar/09/2026

Quality Assurance Department




### Sample Information

Order ID :MTFB20521-01  
 Name :human Histatin 1 peptide  
 Sequence :DSHEKRHHGYRRKFHEKHHSHREFPFYGDYGSNYLYDN  
 Lot. No :MTFB20521-01-260130  
 Pump A :0.1%Trifluoroacetic in 100% water  
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile  
 Total Flow :1ml/min  
 Wavelength :214nm  
 Analytical column type :Kromasil 100-5-C18 (4.6\*250mm\*5 μm)  
 Dissolution method :100%H<sub>2</sub>O  
 Inj. Volume : 15ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	15
30.00	Pumps	B.Conc	45
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	15
50.00	Controller	Stop	

### Chromatogram

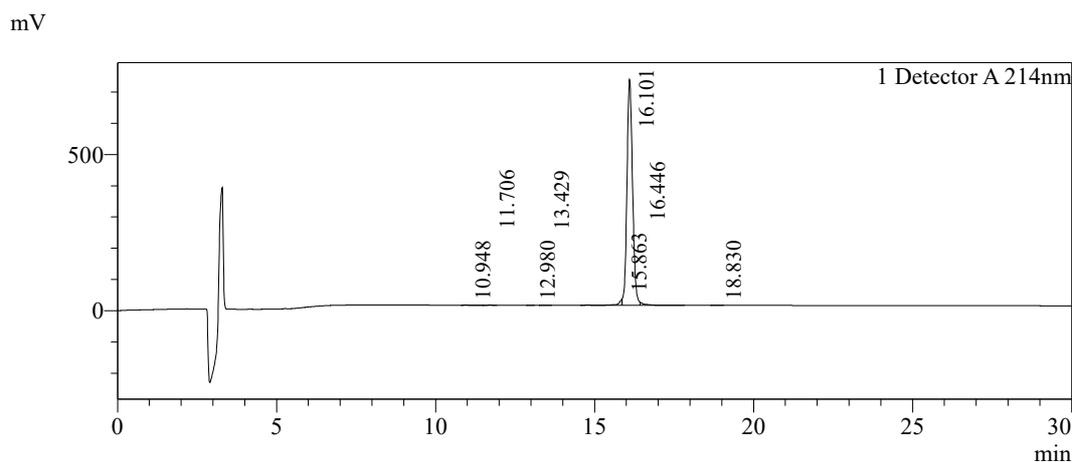


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	10.948	6709	779	0.074
2	11.706	5694	565	0.063
3	12.980	1254	170	0.014
4	13.429	2507	242	0.028
5	15.863	153523	19674	1.689
6	16.101	8815355	722387	96.993
7	16.446	101564	9364	1.117
8	18.830	2072	182	0.023
Total		9088678	753363	100.000

### MS Spectrum

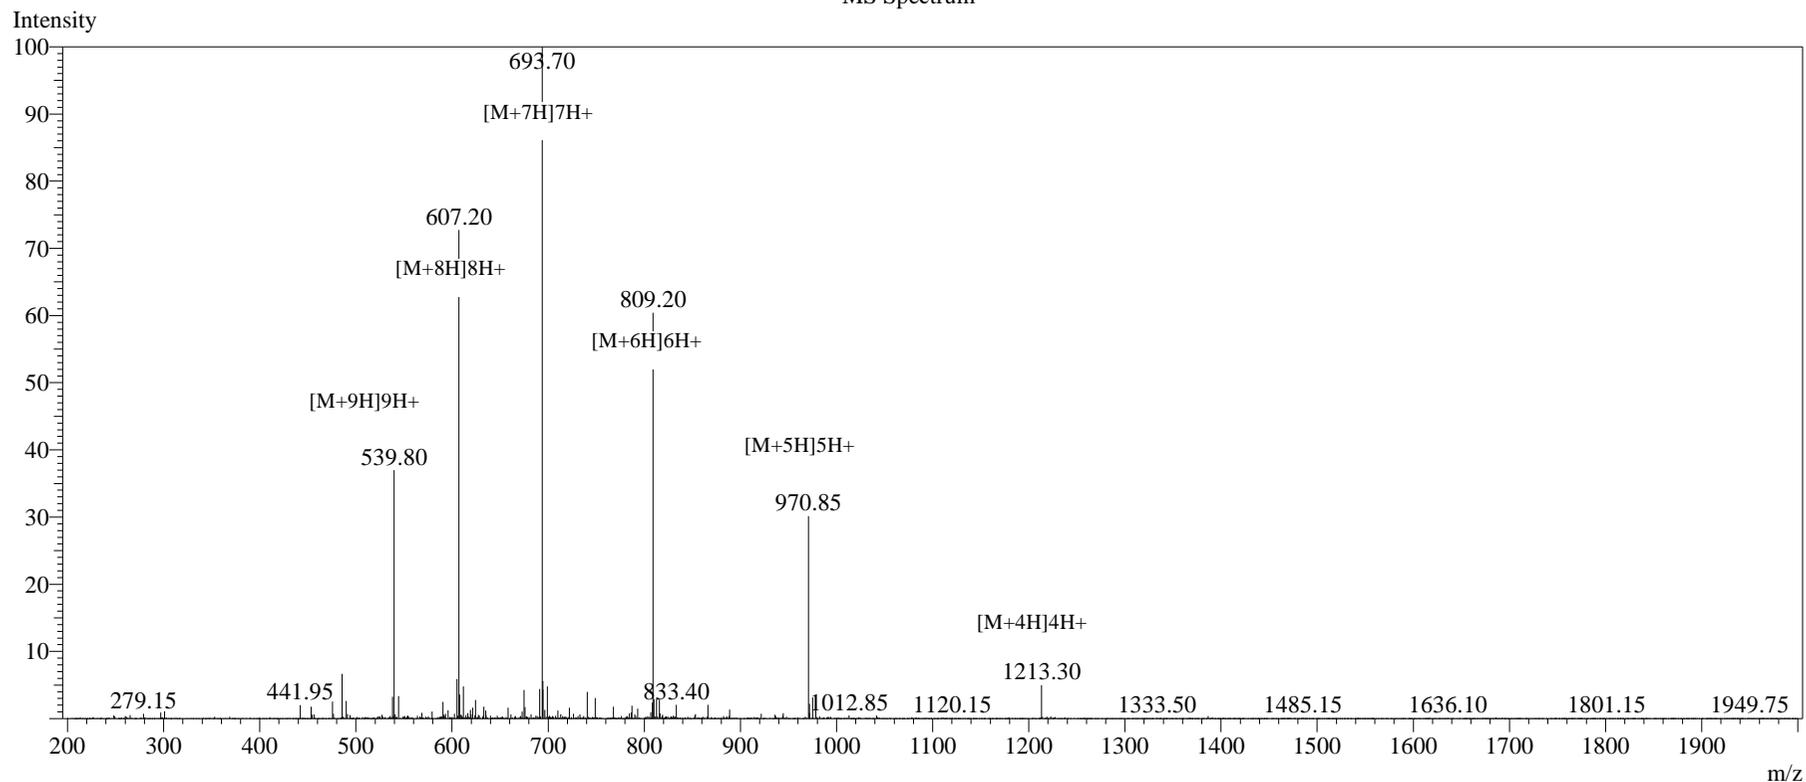

### Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2026/03/05 15:55:00	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% MEOH

Order ID	:MTFB20521-01
Name	:human Histatin 1 peptide
Sequence	:DSHEKRHHGYRRKFHEKHHSHREFPFYGDYGSNYLYDN
Lot.No	:MTFB20521-01-260130
Theoretical	:4848.13
Observed	:4848.90