


CERTIFICATE OF ANALYSIS

Product Name	IKVAV peptide, Cat.#: 319187
Lot No.	MTFA31865-3-0920
Sequence	IKVAV
Dissolution condition	100%H2O
Length	5AA
Modification	N/A
Molecular Weight (MW)	528.70
Storage	-20°C

Test Items	Specifications	Results
MW by MS	528.70	Conforms
Purity by HPLC	>90%	96.433%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	200mg	50.0mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Sep/23/2024




Sample Information

Order ID :MTFA31865-3
 Name :IKVAV peptide
 Sequence :IKVAV
 Lot. No :MTFA31865-3-0920
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Kromasil 100-5-C18 (4.6*250mm*5 µm)
 Dissolution method :100%H2O
 Inj. Volume : 15ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	15
30.00	Pumps	B.Conc	45
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	15
50.00	Controller	Stop	

Chromatogram

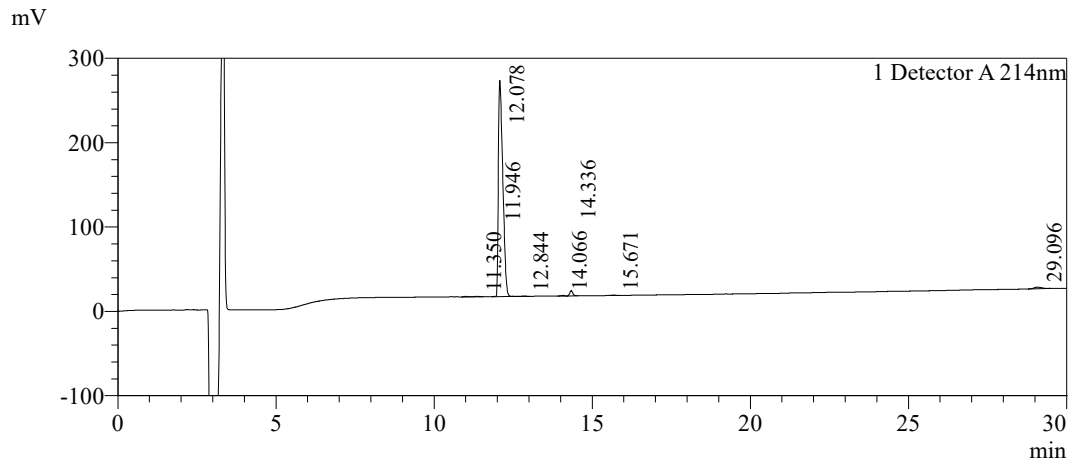


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	11.350	8120	576	0.313
2	11.946	818	202	0.032
3	12.078	2501823	256436	96.433
4	12.844	3661	335	0.141
5	14.066	3995	637	0.154
6	14.336	41199	6069	1.588
7	15.671	3832	541	0.148
8	29.096	30918	1774	1.192
Total		2594366	266570	100.000

MS Spectrum

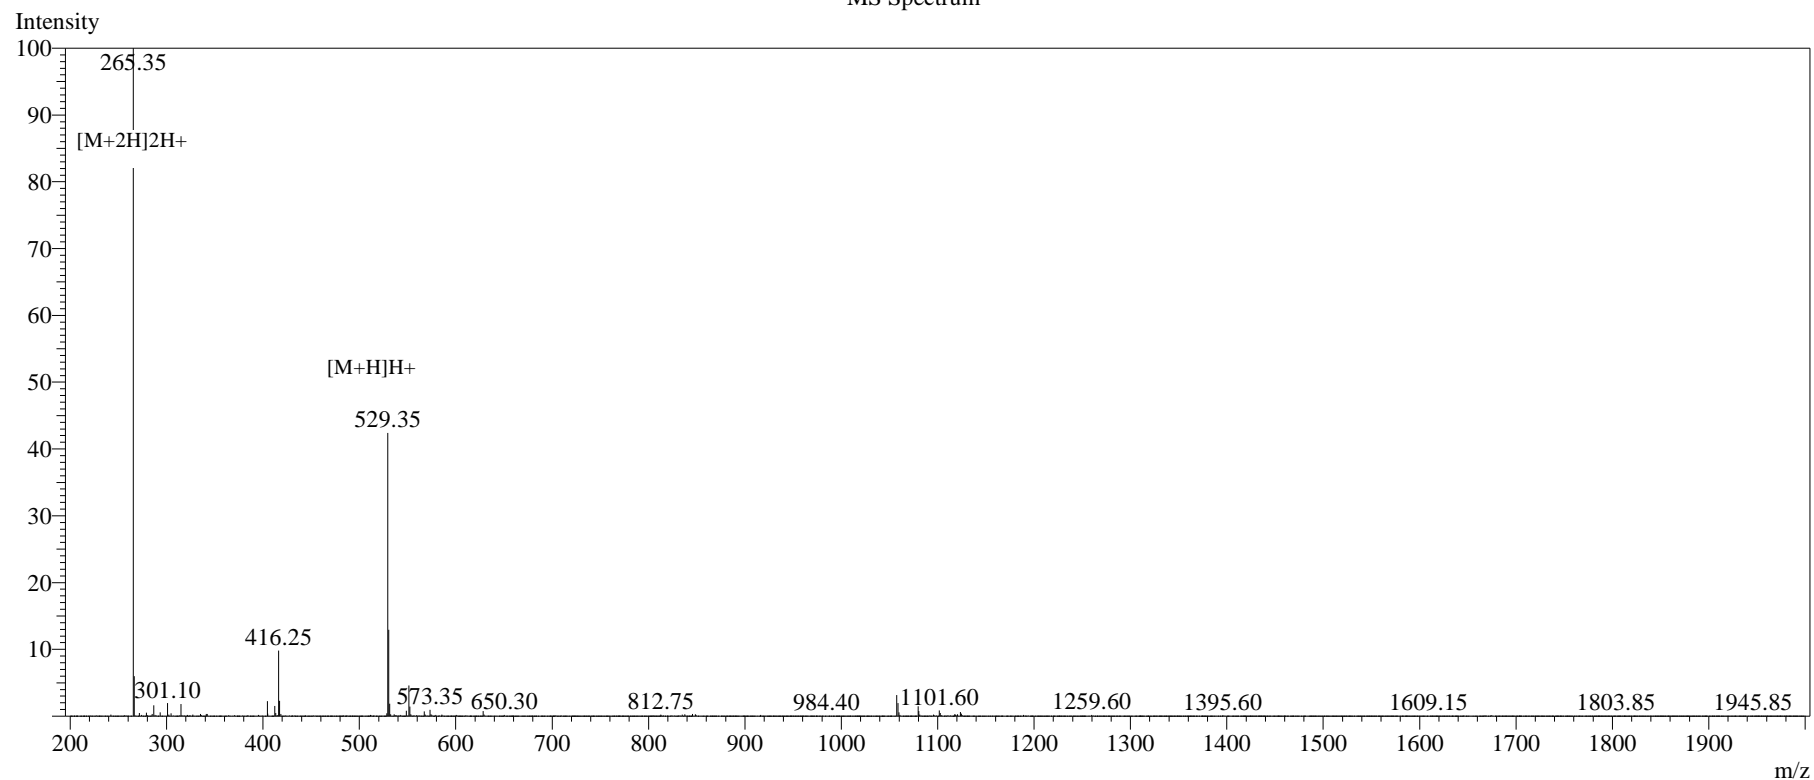

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/09/21 13:34:20	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% MEOH

Order ID	:MTFA31865-3
Name	:IKVAV peptide
Sequence	:IKVAV
Lot.No	:MTFA31865-3-0920
Theoretical	:528.70
Observed	:528.70