
CERTIFICATE OF ANALYSIS

Product Name	Leucocin A (LeuA) Cat.#: 310007
Lot No.	GT30974-5-1218
Sequence	KYYGNGVHCTKSGCSVNWGEAFSAGVHRLANGGNGFW
Dissolution condition	100%H ₂ O
Length	37AA
Modification	N/A
Molecular Weight (MW)	3932.31
Storage	-20°C

Test Items	Specifications	Results
MW by MS	3932.76	Conforms
Purity by HPLC	>95%	95.108%
Peptide Content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	5mg	5.0mg

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

JAN/24/2018




Sample Information

Order ID :GT30974-5
 Name :N/A
 Sequence :KYYGNGVHCTKSGCSVNWGEAFSAGVHRLANGGNGFW
 Lot. No :GT30974-5-1218
 Pump A :0.1% Trifluoroacetic in 100% water
 Pump B :0.1% Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :SHIMADZU Inertsil ODS-SP(4.6*250mm*5um)
 Dissolution method :100% H2O
 Inj. Volume : 60ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	2
30.00	Pumps	B.Conc	65
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	2
50.00	Controller	Stop	

Chromatogram

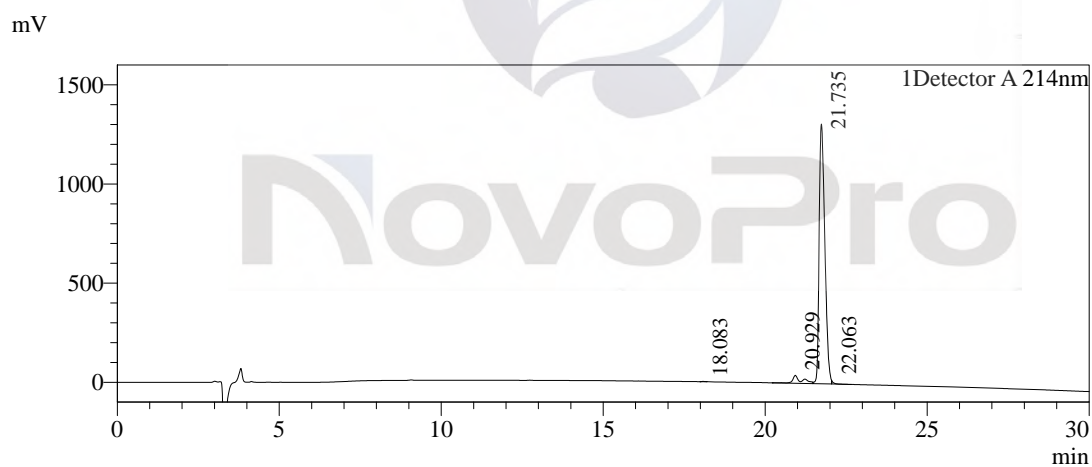


Peak Table


Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	18.083	8459	1442	0.050
2	20.929	750591	40289	4.476
3	21.735	15948147	1310434	95.108
4	22.063	61253	15967	0.365
Total		16768450	1368132	100.000

MS Spectrum

Positive Intensity

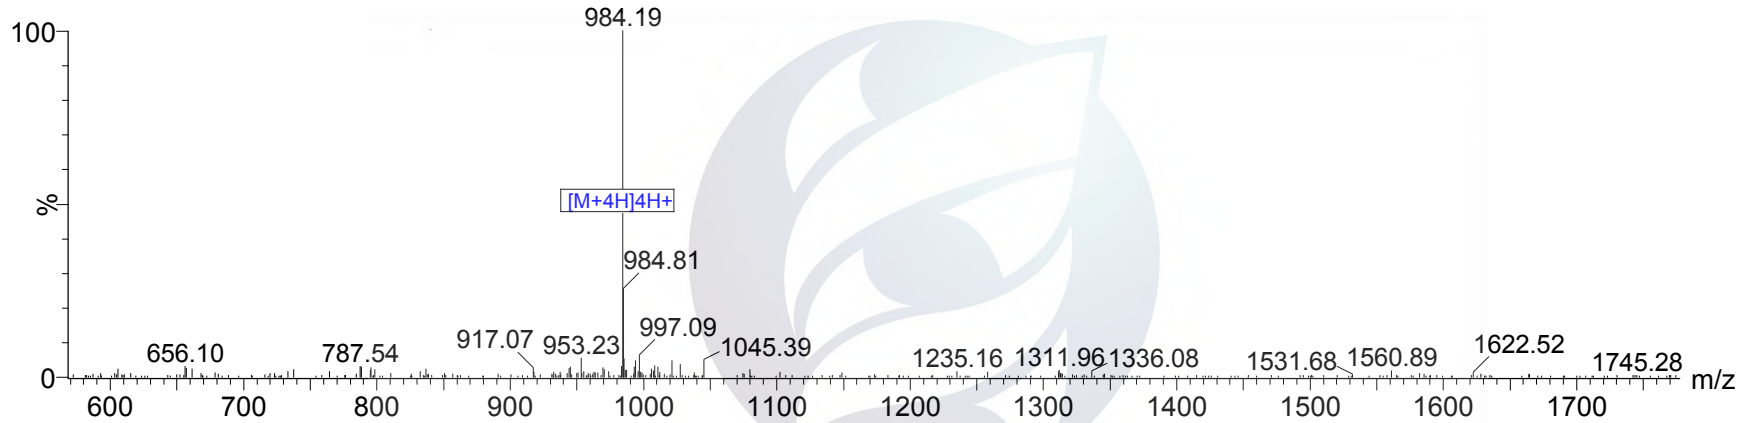

Dissolution method	:5%HAC+8%ACN+87%H2O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2018/1/19 10:38:55	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H2O/50%MEOH
Order ID	:GT30974-5				
Name	:N/A				
Sequence	:KYYGNGVHCTKSGCSVNWGEAFSAGVHRLANGGNGFW				
Lot.No	:GT30974-5-1218				
Theoretical	:3932.31				
Observed	:3932.76				