


**CERTIFICATE OF ANALYSIS**

<b>Product Name</b>	Miraculin (1-20)(Cat.#311434)
<b>Lot No.</b>	GTA33809-0110
<b>Sequence</b>	DSAPNPVLDIDGKLRGTN
<b>Dissolution condition</b>	100%H <sub>2</sub> O
<b>Length</b>	20AA
<b>Modification</b>	N/A
<b>Molecular Weight (MW)</b>	2112.2
<b>Storage</b>	-20°C

<b>Test Items</b>	<b>Specifications</b>	<b>Results</b>
<b>MW by MS</b>	2112.2	Conforms
<b>Purity by HPLC</b>	>95%	95.053%
<b>Peptide Content</b>	N/A	N/A
<b>Moisture content</b>	N/A	N/A
<b>Acetic acid content</b>	N/A	N/A
<b>Appearance</b>	White to off-white lyophilized powder	Conforms
<b>Quantity</b>	10mg	5.0mg*2

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



30/Jan/2021


Quality Assurance Department



### Sample Information

Order ID :GTA33809  
 Name :N/A  
 Sequence :FAEPLPSEEEGESYSKEVPEMEKRYGGFM  
 Lot. No :GTA33809-1110  
 Pump A :0.1% Trifluoroacetic in 100% water  
 Pump B :0.1% Trifluoroacetic in 100% acetonitrile  
 Total Flow :1ml/min  
 Wavelength :214nm  
 Analytical column type :YMC-Triart C18(4.6\*250mm\*5um)  
 Dissolution method :100% H2O  
 Inj. Volume : 65ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	20
25.00	Pumps	B.Conc	45
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	20
50.00	Controller	Stop	

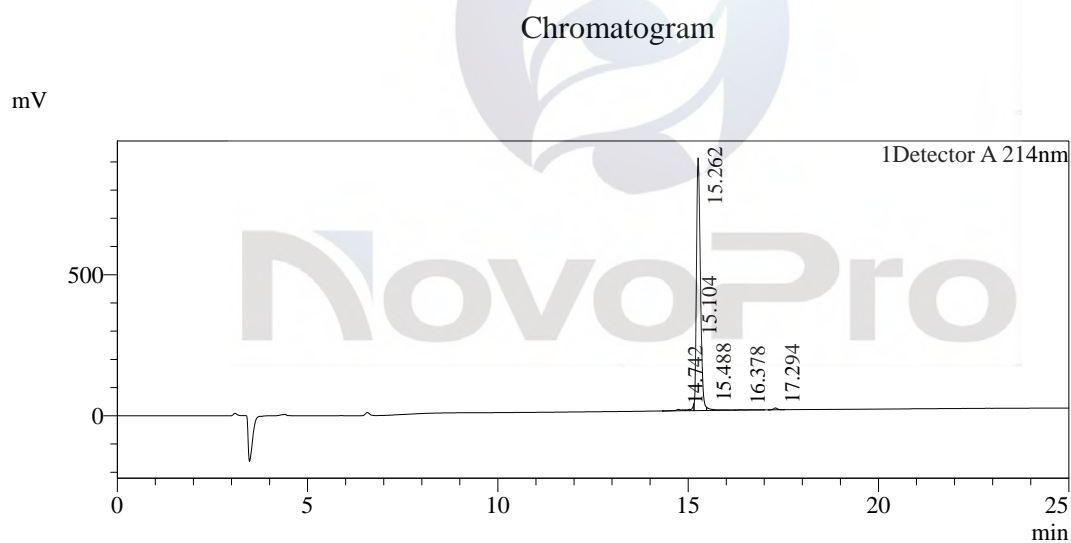


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	14.742	57854	5102	0.858
2	15.104	88461	7459	1.312
3	15.262	6407535	895408	95.053
4	15.488	110710	11475	1.642
5	16.378	29768	1375	0.442
6	17.294	46654	6448	0.692
Total		6740982	927267	100.000

MS Spectrum

Positive Intensity

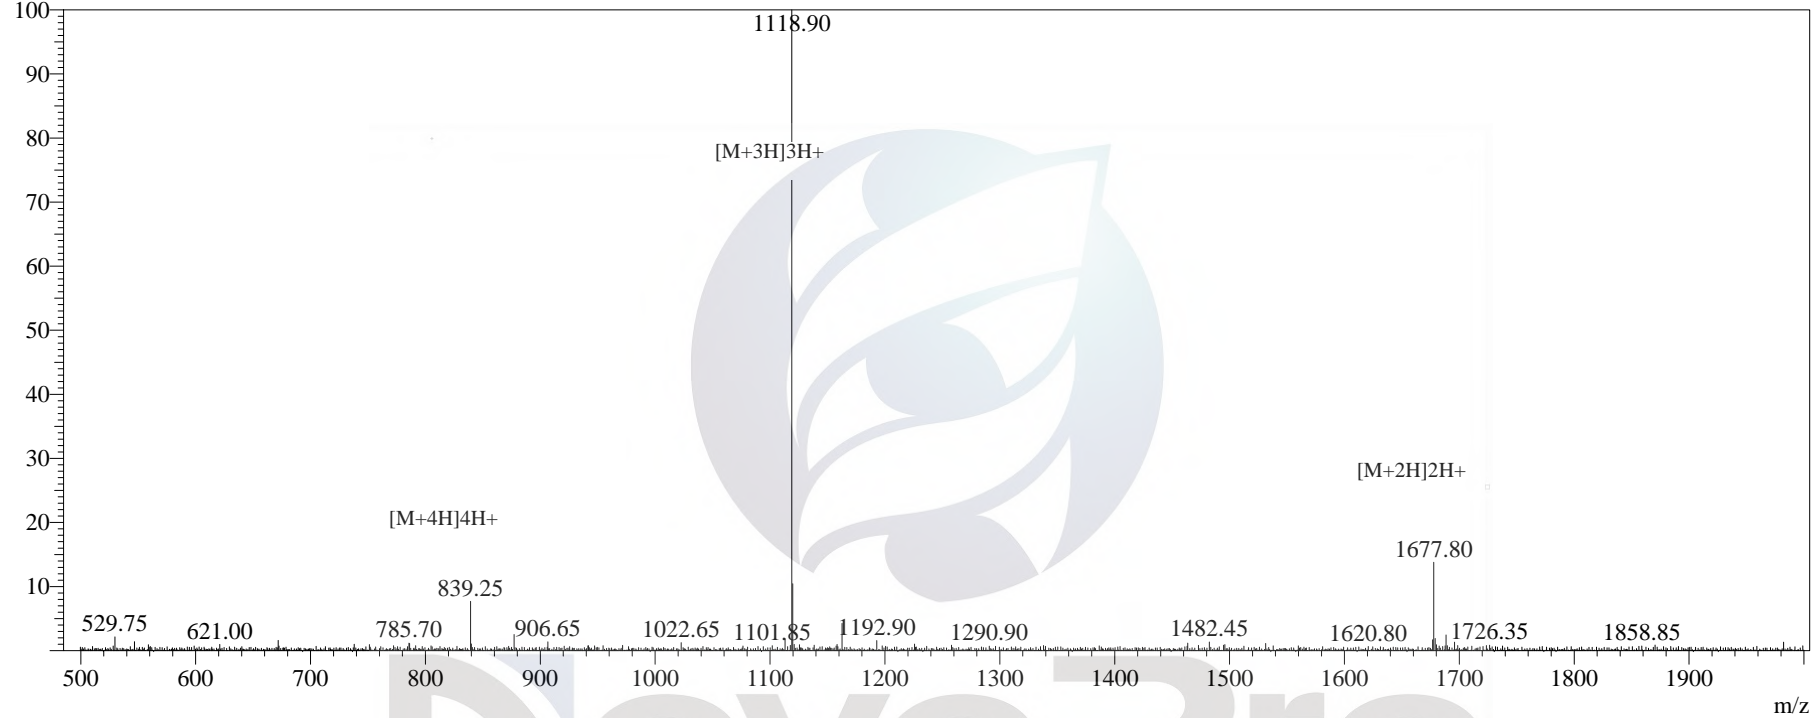

Sample Information

Dissolution method	:5% HAC+8% ACN+87% H2O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2021/12/29 15:45:55	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H2O/50% MEOH

Order ID	:GTA33809
Name	:N/A
Sequence	:FAEPLPSEEEGESYSKEVPEMEKRYGGFM
Lot.No	:GTA33809-1110
Theoretical	:3353.63
Observed	:3353.70