

CERTIFICATE OF ANALYSIS

Product Name	RVG29 peptide, Cat.#: 319149
Lot No.	MTFA31422-0531
Sequence	YTIWMPENPRPGTPCDIFTNSRGKRASNG
Dissolution condition	100%H ₂ O
Length	29AA
Modification	N/A
Molecular Weight (MW)	3266.63
Storage	-20°C

Test Items	Specifications	Results
MW by MS	3267.00	Conforms
Purity by HPLC	>95%	95.176%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	20mg	5.0mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Jun/20/2024




Sample Information

Order ID :MTFA31422
 Name :RVG29 peptide
 Sequence :YTIWMPENPRPGTTPCDIFTNSRGKRASNG
 Lot. No :MTFA31422-0531
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Kromasil 100-5-C18 (4.6*250mm*5 μm)
 Dissolution method :100%H2O

Inj. Volume	Module	Action	Value
30ul			
Time	Module	Action	Value
0.01	Pumps	B.Conc	20
30.00	Pumps	B.Conc	50
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	20
50.00	Controller	Stop	


Chromatogram

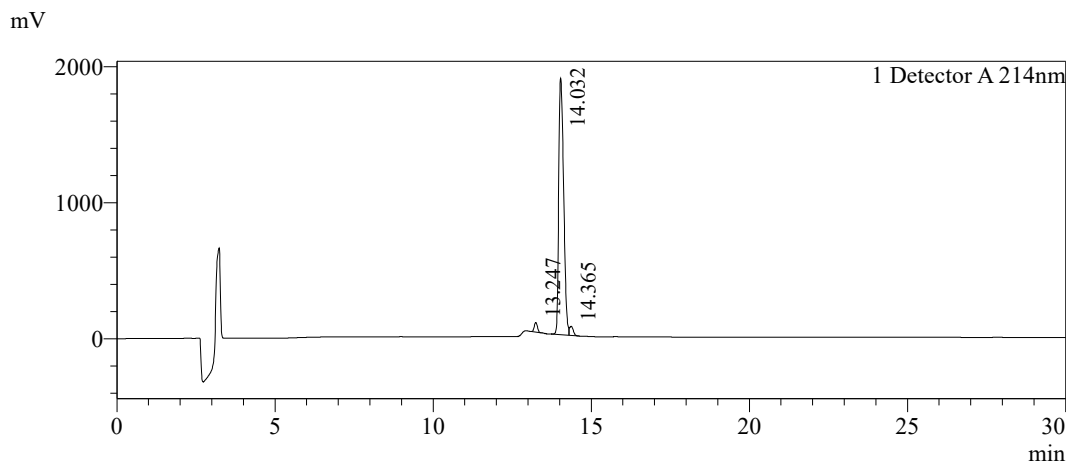

Peak Table

Detector A 214nm				
Peak#	Ret. Time	Area	Height	Area%
1	13.247	495567	71424	2.301
2	14.032	20493853	1884056	95.176
3	14.365	543231	68043	2.523
Total		21532651	2023523	100.000

MS Spectrum

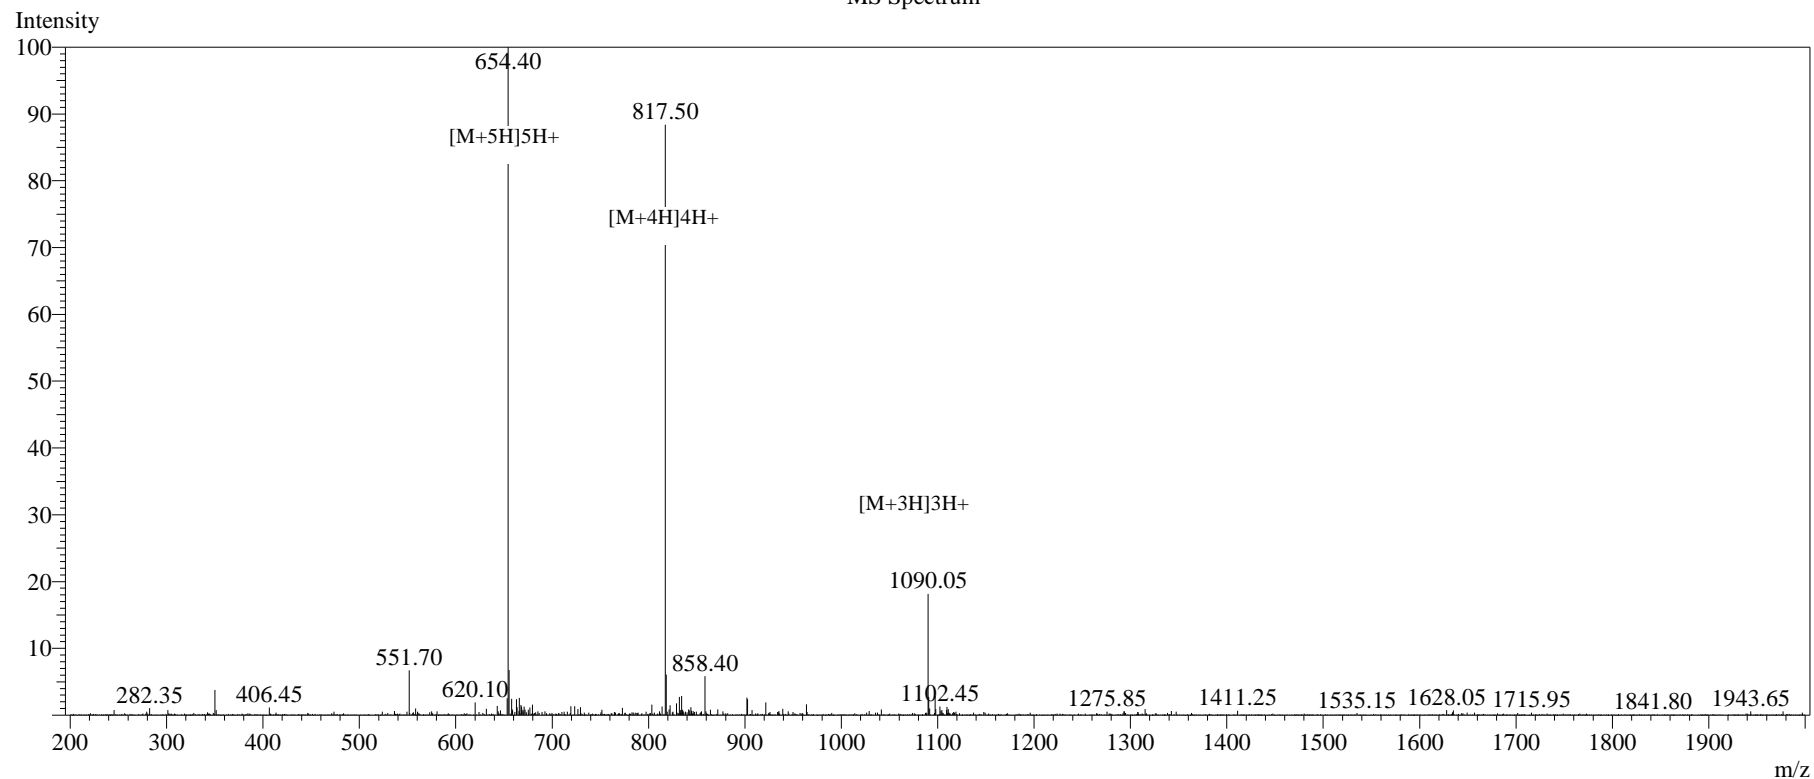

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/06/18 15:37:58	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% MEOH

Order ID	:MTFA31422
Name	:RVG29 peptide
Sequence	:YTIWMPENPRPGTPCDIFTNSRGKRASNG
Lot.No	:MTFA31422-0531
Theoretical	:3266.63
Observed	:3267.00