

CERTIFICATE OF ANALYSIS

Product Name	Rusalatide/TP508, Cat.#: 319711 (TFA removed)
Lot No.	MTFB20825-260507
Sequence	AGYKPDEGKRGDACEGDSGGPFV (Acetate Salt)
Dissolution condition	100%H ₂ O
Modification	Acetate salt
Molecular Weight (MW)	2312.43
Storage	-20°C

Test Items	Specifications	Results
MW by MS	2312.60	Conforms
Purity by HPLC	>95%	95.018%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Peptide content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	1000.0mg	20.0mg*50

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by: 
Quality Assurance Department

Jun/11/2026




Sample Information

Order ID :MTFB20825
 Name :Rusalatide/TP508, Cat.#: 319711 (TFA removed)
 Sequence :AGYKPDEGKRGDACEGDSGGPFV (Acetate Salt)
 Lot. No :MTFB20825-260507
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Kromasil 100-5-C18 (4.6*250mm*5 μm)
 Dissolution method :100%H2O
 Inj. Volume : 30ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	15
30.00	Pumps	B.Conc	45
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	15
50.00	Controller	Stop	

Chromatogram

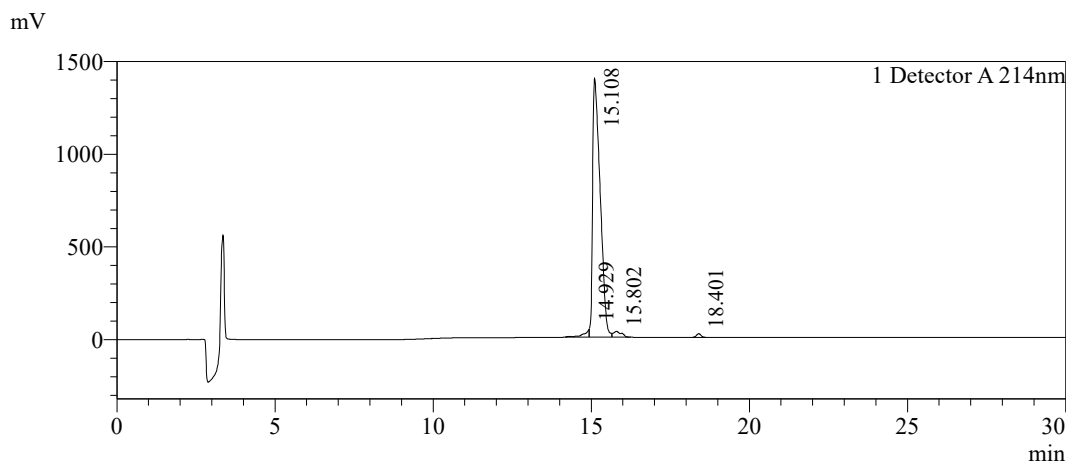


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	14.929	462237	40348	1.889
2	15.108	23251720	1394307	95.018
3	15.802	567709	31436	2.320
4	18.401	189226	19464	0.773
Total		24470892	1485555	100.000

MS Spectrum

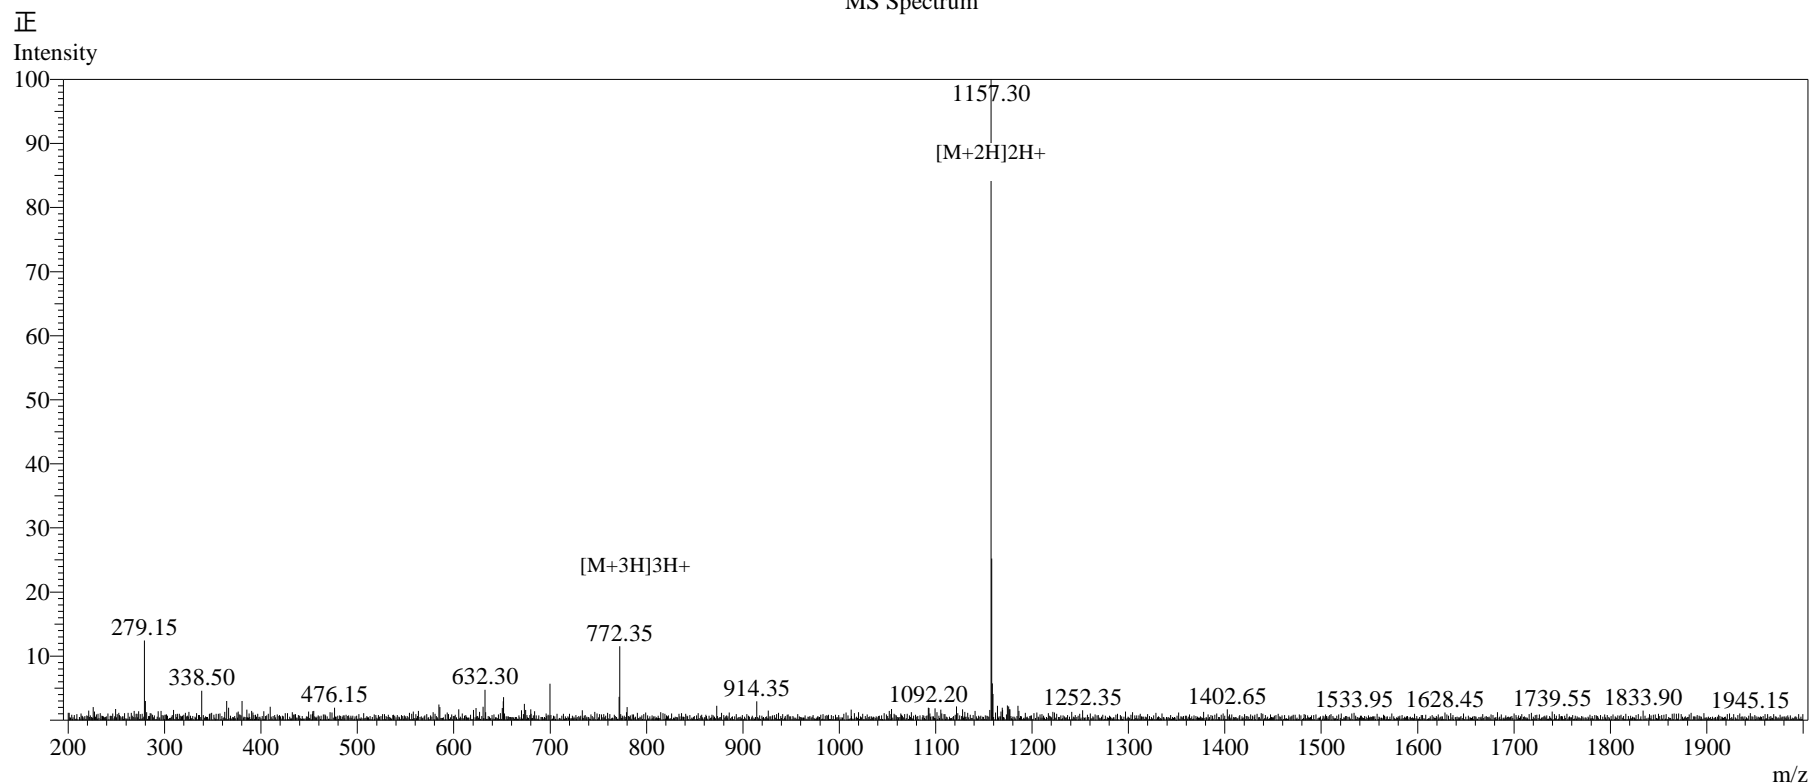

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2026/06/09 10:31:09	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% MEOH

Order ID	:MTFB20825
Name	:Rusalatide/TP508, Cat.#: 319711 (TFA removed)
Sequence	:AGYKPDEGKRGDACEGDSGGPFV(Acetate Salt)
Lot.No	:MTFB20825-260507
Theoretical	:2312.43
Observed	:2312.60