

CERTIFICATE OF ANALYSIS

Product Name	Temporin L peptide, Cat.# 305491
Lot No.	MTFA30001-2-0308
Sequence	FVQWFSKFLGRIL-NH2
Dissolution condition	100%H2O
Length	13AA
Modification	N/A
Molecular Weight (MW)	1639.98
Storage	-20°C

Test Items	Specifications	Results
MW by MS	1640.38	Conforms
Purity by HPLC	95.0%	95.837%
Peptide Content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	10mg	5.0mg*2

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Mar/14/2023




Sample Information

Order ID :MTFA30001-2
 Name :Temporin L peptide, Cat.# 305491
 Sequence :FVQWFSKFLGRIL-NH2
 Lot. No :MTFA30001-2-0308
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Shim-pack GIST C18(4.6*250mm*5um)
 Dissolution method :100%H2O
 Inj. Volume : 30ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	30
30.00	Pumps	B.Conc	60
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	30
50.00	Controller	Stop	

Chromatogram

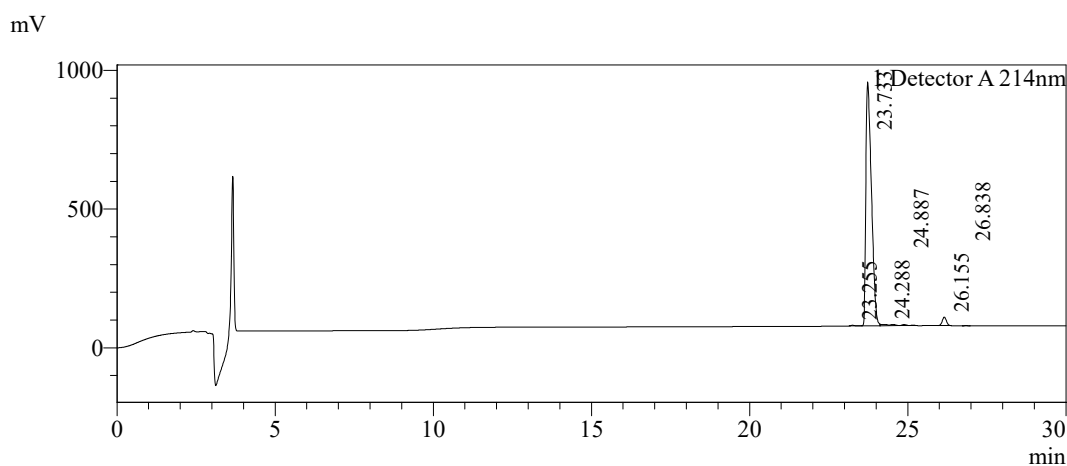


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	23.255	21401	2425	0.190
2	23.733	10783586	878966	95.837
3	24.288	120055	4722	1.067
4	24.887	47780	3919	0.425
5	26.155	273775	30325	2.433
6	26.838	5437	775	0.048
Total		11252035	921131	100.000

MS Spectrum

Positive Intensity

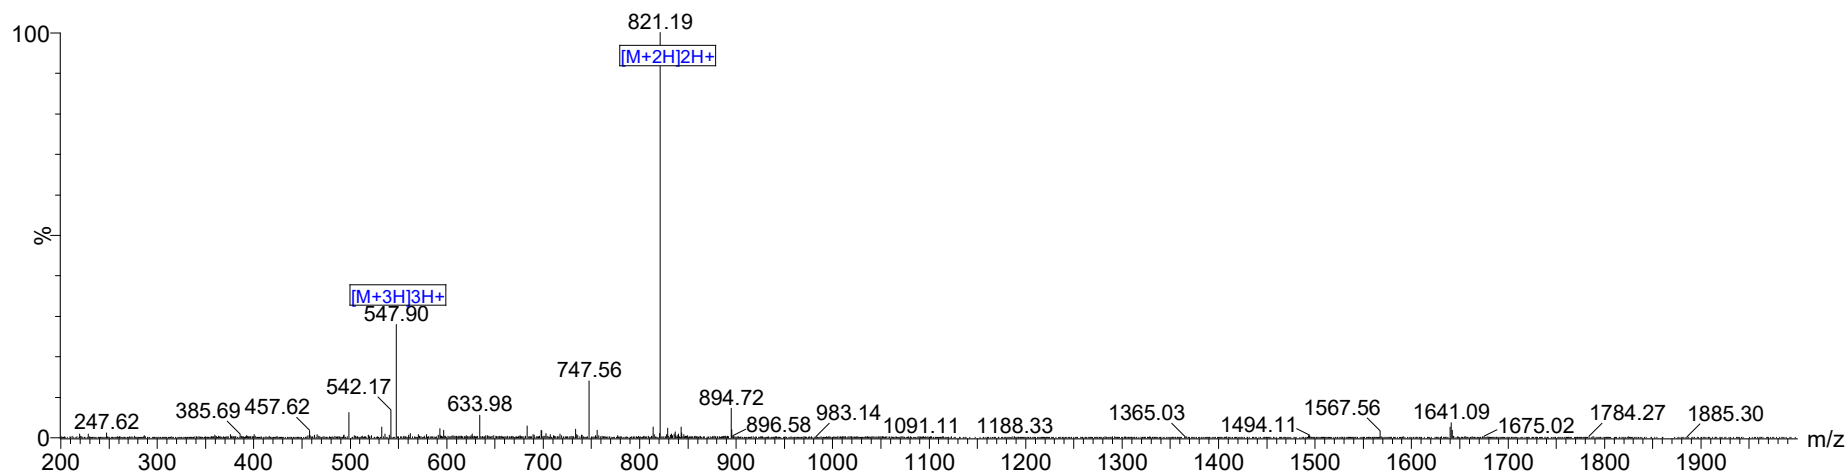

Dissolution method	:15%ACN+85%H2O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2023/3/13 23:23:29	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H2O/50%MEOH

Order ID : MTF30001-2
 Name : Temporin L peptide, Cat.# 305491
 Sequence : FVQWFSKFLGRIL-NH2
 Lot.No : MTF30001-2-0308
 Theoretical : 1639.98
 Observed : 1640.38