

CERTIFICATE OF ANALYSIS

Product Name	novispirin G10 peptide, Cat.#: 318936 (TFA removed)
Lot No.	MTFB20705-01-260721
Sequence	KNLRRRIIRKGIHIIKKYG (Acetate salt)
Dissolution condition	100%H2O
Modification	N/A
Molecular Weight (MW)	2206.73
Storage	-20°C

Test Items	Specifications	Results
MW by MS	2206.98	Conforms
Purity by HPLC	95%	98.230%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Peptide content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	40mg	8 x 5mg

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Sep/02/2026

Quality Assurance Department




Sample Information

Name : novispirin G10 peptide, Cat.#: 318936 (TFA removed)
 Sequence : KNLRRIIRKGIHIKKYG
 Lot. No : MTFB20705-01-260721
 Pump A : 0.1%Trifluoroacetic in 100% water
 Pump B : 0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow : 1ml/min
 Wavelength : 214nm
 Analytical column type : Kromasil 100-5-C18 (4.6*250mm*5 um)
 Dissolution method : 100%H₂O
 Inj. Volume : 15ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	45
30.00	Pumps	B.Conc	75
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	45
50.00	Controller	Stop	-

Chromatogram

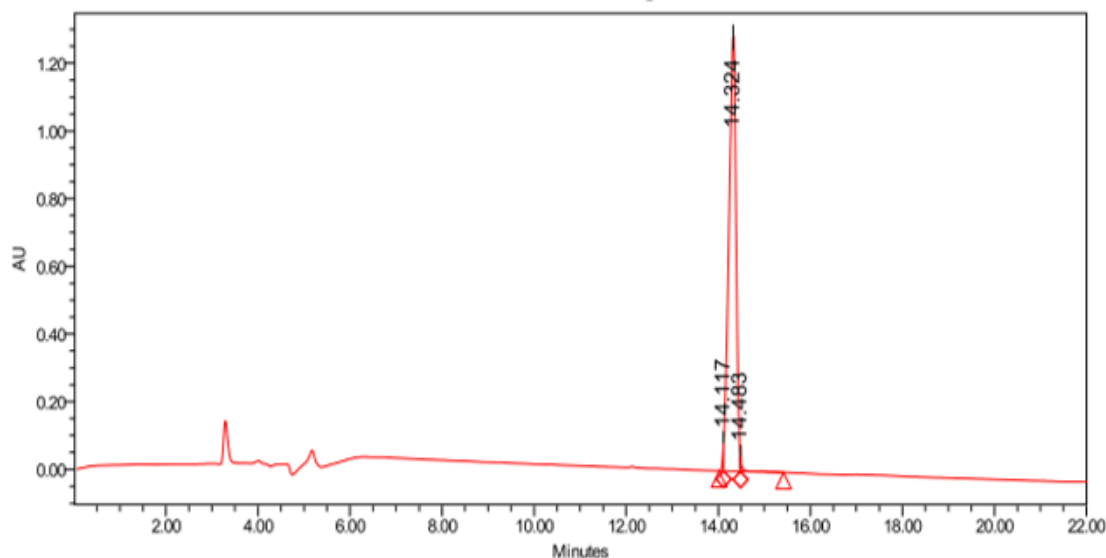


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	14.117	113887	79854	0.813
2	14.324	13759098	1296962	98.230
3	14.483	134065	41314	0.957
Total	-	14007050	1418130	100

MS Spectrum

Scan ES+
3.16e7

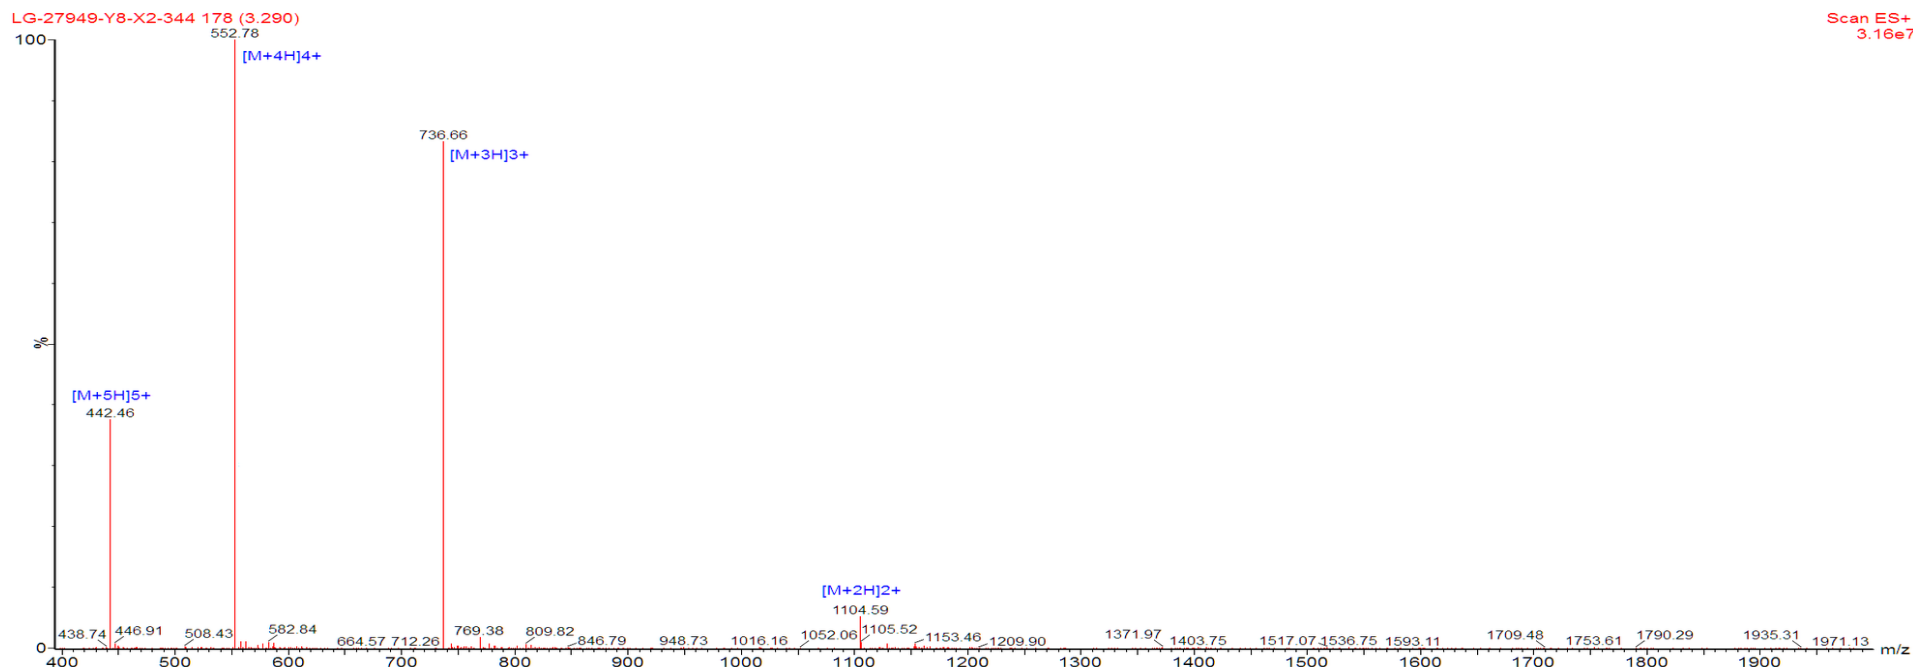

Sample Information

Dissolution method	: 15%ACN+85%H2O	Interface	: ESI	Prerod Bias	: +4.5kv
Date Acquired	: 2026/05/22 09:35:06	Nebulizing Gas Flow	: 1.50L/min	Detector	: -0.2kv
Injection Volume	: 0.2ul	CDL Temp	: 250°C	T.Flow	: 0.2ml/min
Block Temp	: 200	CDL Volt	: 0v	B.conc	: 50%H2O/50%MEOH
Name	: novispirin G10 peptide, Cat.#: 318936 (TFA removed)				
Sequence	: KNLRRIIRKGIHIKKYG				
Lot.No	: MTFB20705-01-260721				
Theoretical	: 2206.73				
Observed	: 2206.98				