

---

**CERTIFICATE OF ANALYSIS**

<b>Product Name</b>	self-assembling P11-4, Cat.#: 319744 (TFA removed)
<b>Lot No.</b>	MTFB20583-260225
<b>Sequence</b>	Ac-QQRFWEFEQQ-NH2 (Acetate Salt)
<b>Dissolution condition</b>	2%NH3.H2O+18%ACN+80%H2O
<b>Modification</b>	acetate salt
<b>Molecular Weight (MW)</b>	1595.69
<b>Storage</b>	-20°C

---

<b>Test Items</b>	<b>Specifications</b>	<b>Results</b>
<b>MW by MS</b>	1595.70	Conforms
<b>Purity by HPLC</b>	>95%	95.807%
<b>Endotoxin Content</b>	N/A	N/A
<b>TFA solubility</b>	N/A	N/A
<b>Moisture content</b>	N/A	N/A
<b>Acetic acid content</b>	N/A	N/A
<b>Appearance</b>	White to off-white lyophilized powder	Conforms
<b>Quantity</b>	20mg	5.0mg*4

---

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:   
Quality Assurance Department

Mar/02/2026




### Sample Information

Order ID :MTFB20583  
 Name :self-assembling P11-4  
 Sequence :Ac-QQRFWEFEQQ-NH2 (Acetate Salt)  
 Lot. No :MTFB20583-260225  
 Pump A :0.1%Trifluoroacetic in 100% water  
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile  
 Total Flow :1ml/min  
 Wavelength :214nm  
 Analytical column type :Kromasil 100-5-C18 (4.6\*250mm\*5 μm)  
 Dissolution method :2%NH3.H2O+18%ACN+80%H2O  
 Inj. Volume : 50ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	20
30.00	Pumps	B.Conc	50
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	20
50.00	Controller	Stop	

### Chromatogram

mV

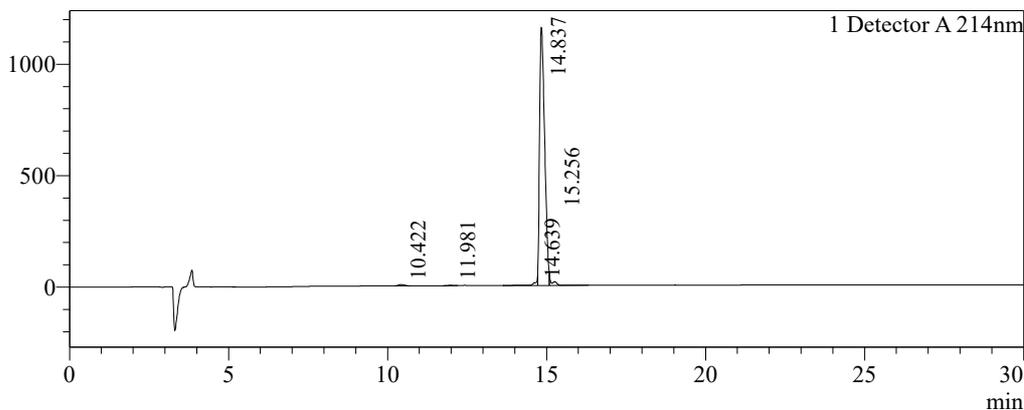


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	10.422	72931	6141	0.541
2	11.981	22688	2368	0.168
3	14.639	183933	12390	1.365
4	14.837	12913666	1156150	95.807
5	15.256	285560	16833	2.119
Total		13478779	1193883	100.000

MS Spectrum

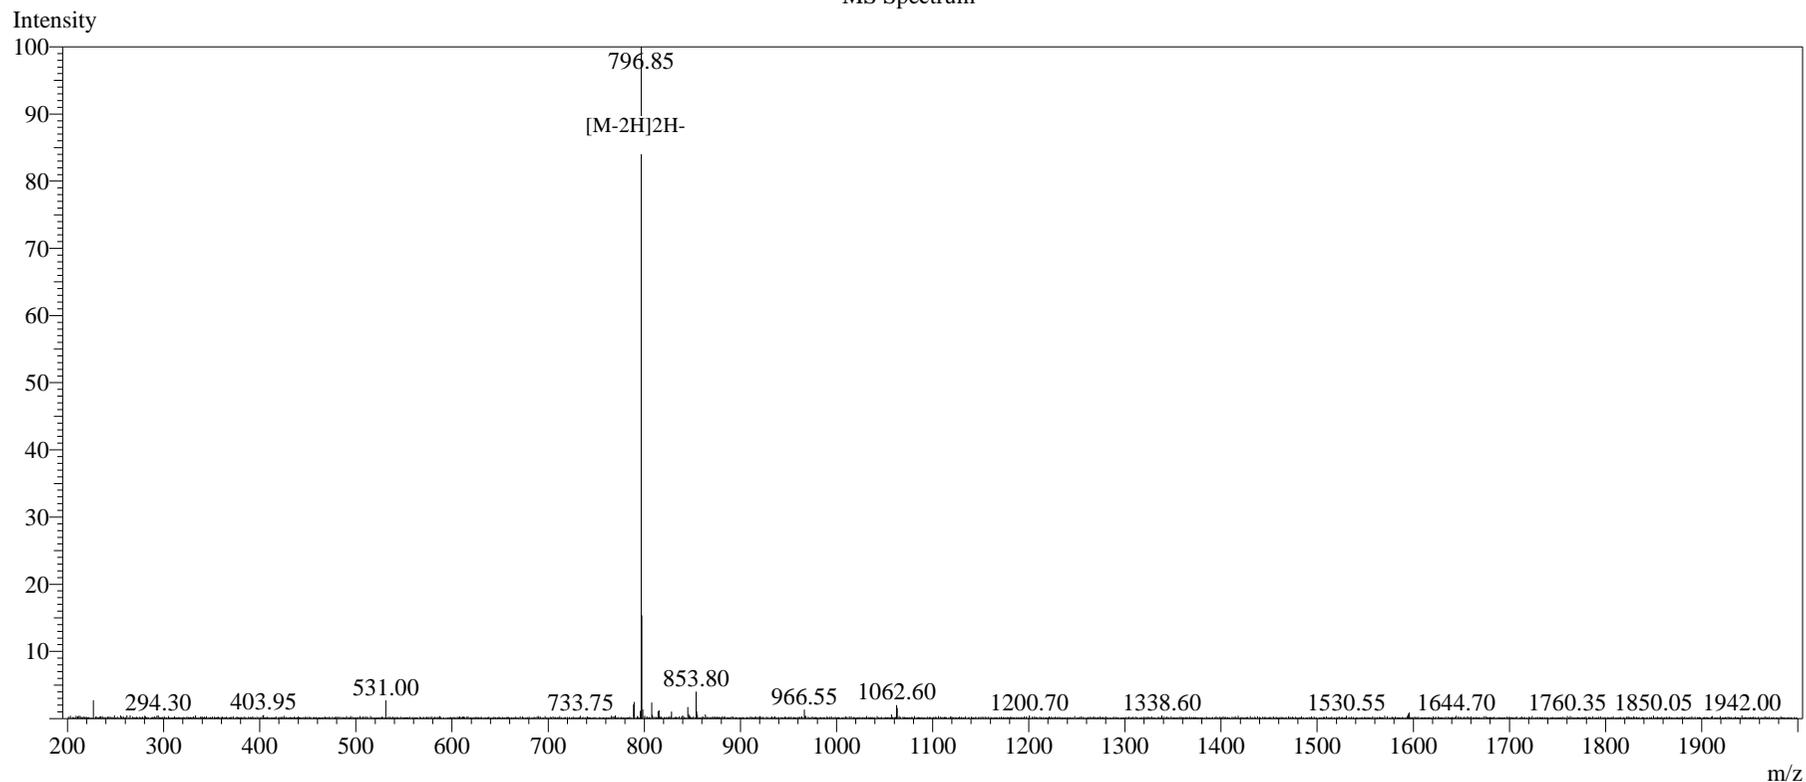

Sample Information

Dissolution method	:2% NH <sub>3</sub> .H <sub>2</sub> O+18% ACN+80% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2026/02/26 16:15:08	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% MEOH

Order ID	:MTFB20583
Name	:self-assembling P11-4
Sequence	:Ac-QQRFWEFEQQ-NH <sub>2</sub> (Acetate Salt)
Lot.No	:MTFB20583-260225
Theoretical	:1595.69
Observed	:1595.70