
CERTIFICATE OF ANALYSIS

Product Name	β -Amyloid(16-20), Cat.#: 302802 (TFA removed)
Lot No.	MTFA33575-251112
Sequence	KL VFF (Acetate Salt)
Dissolution condition	100% H ₂ O
Modification	acetate salt
Molecular Weight (MW)	652.82
Storage	-20°C

Test Items	Specifications	Results
MW by MS	652.60	Conforms
Purity by HPLC	>95%	99.753%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	200mg	5.0mg*40

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Nov/17/2025


Quality Assurance Department



Sample Information

Order ID	:MTFA33575		
Name	:β-Amyloid(16-20)		
Sequence	:KLVFF (Acetate Salt)		
Lot. No	:MTFA33575-251112		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 μm)		
Dissolution method	:100%H2O		
Inj. Volume	: 20ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	25
30.00	Pumps	B.Conc	55
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	25
50.00	Controller	Stop	

Chromatogram

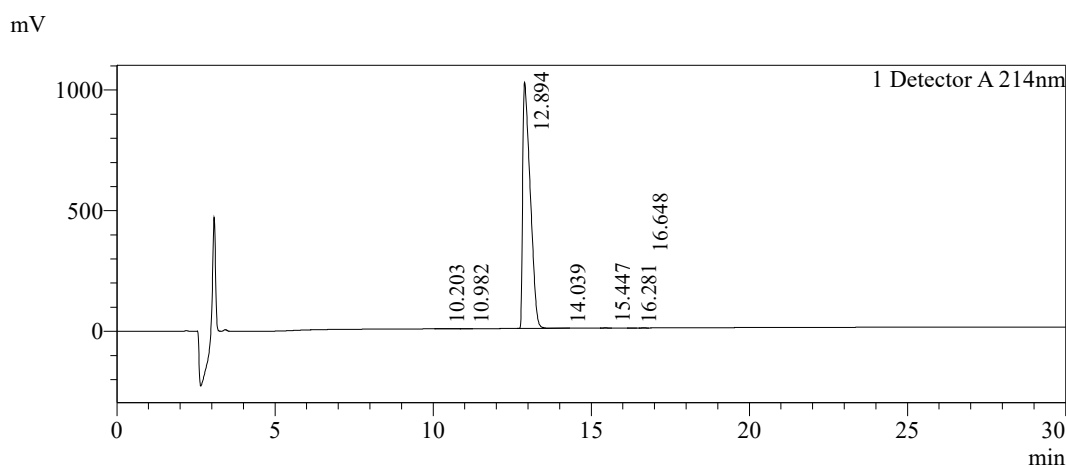


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	10.203	8298	516	0.049
2	10.982	3091	365	0.018
3	12.894	16889668	1019963	99.753
4	14.039	16562	974	0.098
5	15.447	9202	1127	0.054
6	16.281	2225	284	0.013
7	16.648	2479	310	0.015
Total		16931525	1023538	100.000

MS Spectrum

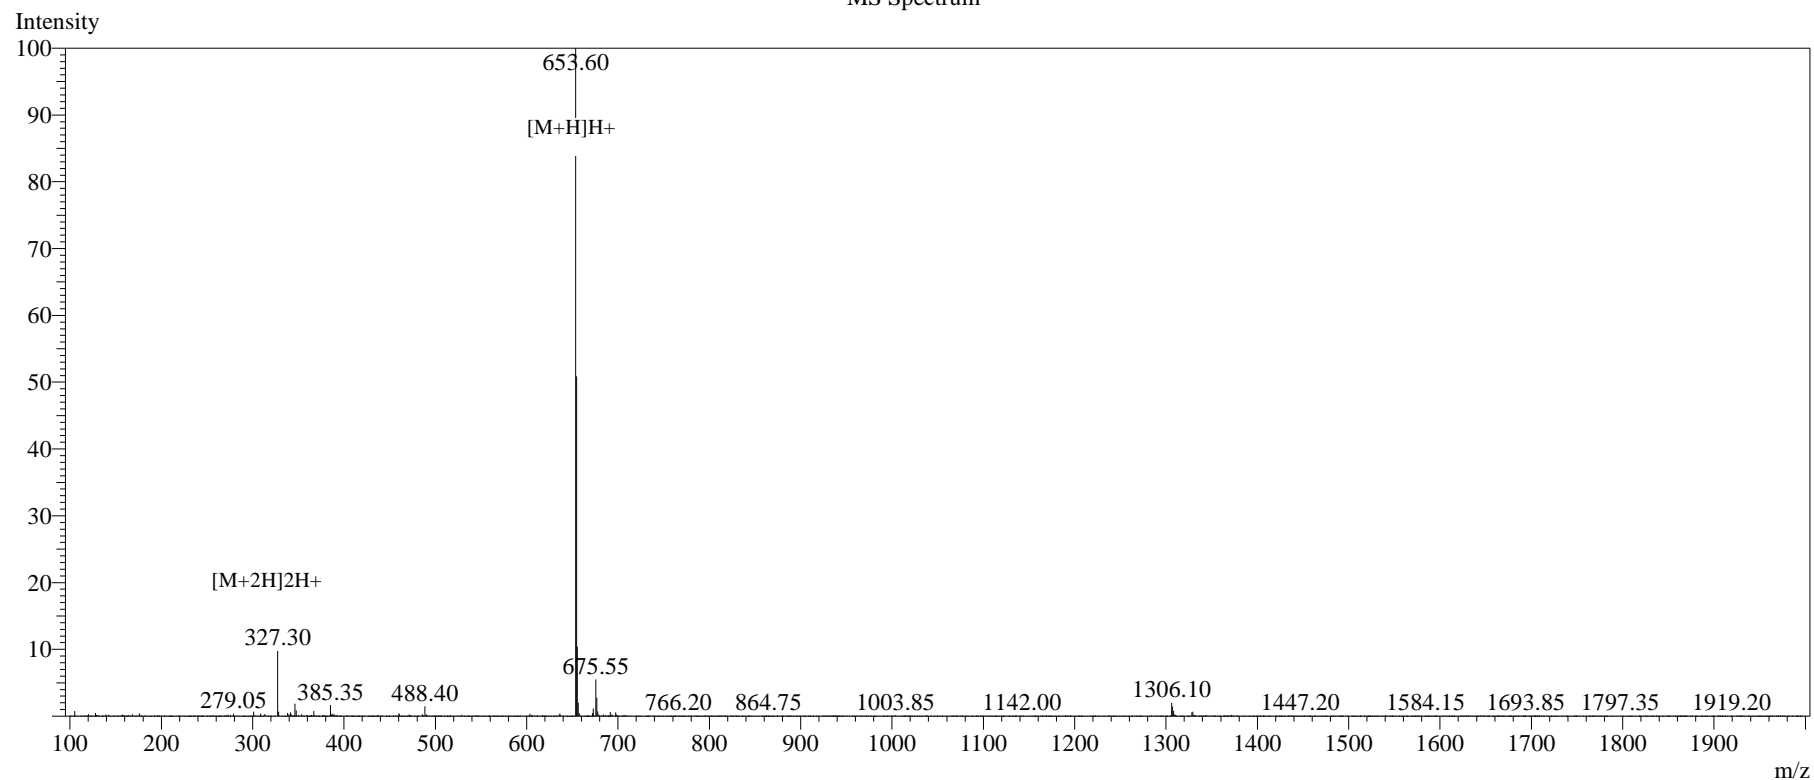

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/11/14 11:14:54	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% ME OH
Order ID	:MTFA33575				
Name	:β-Amyloid(16-20)				
Sequence	:KLVFF(Acetate Salt)				
Lot.No	:MTFA33575-251112				
Theoretical	:652.82				
Observed	:652.60				